

**Agilent Technologies**  
**16533A/34A Digitizing Oscilloscope**  
**Service Guide**

Install this package in the binder that includes  
the Service Guide for the Agilent Technologies 16700 Logic Analysis System.



---

# Service Guide

Publication number 16534-97013

Third edition, September 2000

For Safety information, Warranties, and Regulatory information, see the pages at the end of the book.

© Copyright Agilent Technologies 1987-2000

All Rights Reserved.

---

**Agilent Technologies 16533A 1-GSa/s  
and 16534A 2-GSa/s Digitizing  
Oscilloscope (16700-series Version)**

---

# The Agilent Technologies 16533A/34A Oscilloscope

The Agilent Technologies 16533A/34A Oscilloscope is an oscilloscope module for the Agilent Technologies 16700-series Logic Analysis system, and is designed to extend system troubleshooting capabilities for viewing analog effects on the fastest CMOS, ECL, and TTL logic circuitry.

## Features

- 1 GSa/s digitizing for 250 MHz bandwidth single shot oscilloscope (16533A)
- 2 GSa/s digitizing for 500 MHz bandwidth single shot oscilloscope (16534A)
- 32,768 samples per channel
- Automatic pulse parameters, displays time between markers, acquires until specified time between markers is captured, performs statistical analysis on time between markers
- Lightweight miniprobes

## Service Strategy


The service strategy for this instrument is the replacement of defective assemblies. This service guide contains information for finding a defective assembly by testing and servicing the 16533A/34A Oscilloscope.

This logic analyzer can be returned to Agilent Technologies for all service work, including troubleshooting. Contact your nearest Agilent Technologies Sales Office for more details.

## Application

This service guide applies to an Agilent Technologies 16533/34A module installed in the 16700-series logic analysis system mainframe running operating system A.02.00 or later.

If your mainframe operating system is older than the required version, contact your Agilent Technologies Service Center for newer software before attempting the performance verification procedures in chapter 3.

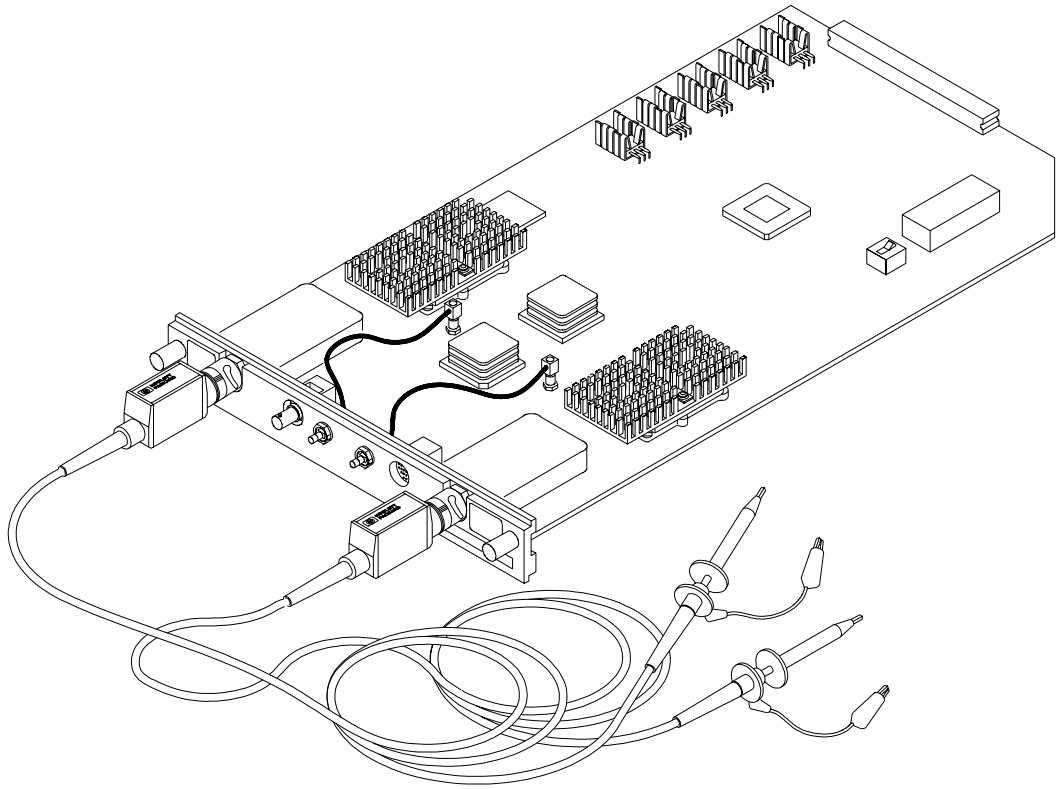

16534e03

**The Agilent Technologies 16533A/34A Oscilloscope**

---

## In This Book

This book is the service guide for the 16533A and 16534A Oscilloscopes and is divided into eight chapters.

Chapter 1 contains information about the oscilloscope and includes accessories, specifications and characteristics, and equipment required for servicing.

Chapter 2 tells how to prepare the oscilloscope for use.

Chapter 3 gives instructions on how to test the performance of the oscilloscope.

Chapter 4 contains calibration instructions for the oscilloscope.

Chapter 5 contains self-tests and flowcharts for troubleshooting the oscilloscope.

Chapter 6 tells how to replace assemblies of the oscilloscope and how to return them to Agilent Technologies.

Chapter 7 lists replaceable parts, shows an exploded view, and gives ordering information.

Chapter 8 explains how the oscilloscope works and what the self-tests are checking.

---

# Contents

## 1 General Information

Accessories	1-2
Specifications	1-3
Environmental Characteristics	1-4
Recommended Test Equipment	1-5

## 2 Preparing for Use

To inspect the module	2-2
To prepare the mainframe	2-3
To configure the 16533/34A module	2-4
To reconfigure a multocard module into single card modules	2-5
To turn on the system	2-6
To test the module	2-6

## 3 Testing Performance

To Perform the Self-tests	3-3
Perform the power-up tests	3-3
Perform the self-tests	3-4
To test the input resistance	3-5
Set up the equipment	3-5
Set up the oscilloscope	3-6
Connect the oscilloscope	3-8
Acquire the data	3-8
Perform an operational accuracy calibration	3-9
To test the voltage measurement accuracy	3-9
Set up the equipment	3-9
Set up the oscilloscope	3-10
Connect the oscilloscope	3-13
Acquire the data	3-13
To test the offset accuracy	3-16
Set up the equipment	3-16
Set up the oscilloscope	3-17
Connect the oscilloscope	3-20
Acquire the zero input data	3-20
Acquire the DC input data	3-22
To test the bandwidth (16533A only)	3-24
Set up the equipment	3-24
Set up the oscilloscope	3-25
Connect the oscilloscope	3-28
Acquire the data	3-28
To test the bandwidth (16534A only)	3-31

## Contents

Set up the equipment	3-31
Set up the oscilloscope	3-32
Connect the oscilloscope	3-35
Acquire the data	3-35
To test the time measurement accuracy	3-38
Set up the equipment	3-38
Set up the oscilloscope	3-39
Connect the oscilloscope	3-42
Acquire the data	3-43
To test the trigger sensitivity (16533A only)	3-46
Set up the equipment	3-46
Set up the oscilloscope	3-47
Connect the oscilloscope	3-50
Acquire the data	3-50
To test the trigger sensitivity (16534A only)	3-53
Set up the equipment	3-53
Set up the oscilloscope	3-54
Connect the oscilloscope	3-57
Acquire the data	3-57
Performance Test Record	3-60
<b>4 Calibrating and Adjusting</b>	
Oscilloscope calibration	4-2
Multicard oscilloscope calibration	4-2
To calibrate the oscilloscope	4-3
Set up the equipment	4-3
Self Cal calibrations	4-4
Protect the operational accuracy calibration factors	4-8
Load the default calibration factors	4-8
To deskew the channel-to-channel variations	4-9
<b>5 Troubleshooting</b>	
To use the flowcharts	5-2
To run the self-tests	5-5
To verify the CAL OUTPUT port	5-6
Set up the equipment	5-6
Set up the oscilloscope	5-7
Verify the cal DC output voltages	5-8
Set up the oscilloscope	5-9
Verify the AC CAL OUTPUT	5-10
<b>6 Replacing Assemblies</b>	
To remove the module	6-2



To remove the trigger cable	6-3
To replace the trigger cable	6-4
To remove the attenuator	6-4
To replace the attenuator	6-4
To remove the circuit board	6-5
To replace the circuit board	6-5
To replace the module	6-5
To return assemblies	6-6

## **7 Replaceable Parts**

Replaceable Parts Ordering	7-2
Replaceable Parts List	7-3
Exploded View	7-5

## **8 Theory of Operation**

Block-Level Theory	8-3
Self-Tests Description	8-7
Oscilloscope Tests (PV)	8-7



General Information

Accessories 1-2

Specifications 1-3

Environmental Characteristics 1-4

Recommended Test Equipment 1-5

---

# General Information

This chapter lists the accessories, the specifications and characteristics, and the recommended test equipment.

---

## Accessories

<b>Accessories Supplied</b>	<b>Agilent Part Number</b>	<b>Qty</b>
10:1 probes	10441B	2
BNC miniprobe adapter	5063-2143	1

### **Accessories Available**

Other accessories available for the Agilent Technologies 16533A/34A oscilloscope are listed in the *Accessories for Agilent Logic Analyzers* brochure and the *Accessories for Agilent Oscilloscopes* brochure.

## Specifications

The specifications are the performance standards against which the 16533A/34A Oscilloscope is tested.

**Bandwidth(\*):**

16533A - dc to 250 MHz (realtime, dc coupled)

16534A - dc to 500 MHz (realtime, dc coupled)

**Time Interval Measurement Accuracy(\*)**(1)**:** +/-[(0.005% of delta t) + (2 x 10e-6 x delay setting) + 100 ps]

**DC Offset Accuracy(\*):** +/- (1.0% of channel offset + 2.0% of full scale)

**Voltage Measurement Accuracy(\*):** +/- (1.65% of full scale + offset accuracy)

**Trigger Sensivity(\*):**

dc to 50 MHz:	0.50 div
50 MHz to 250 MHz (16533A):	1.00 div
50 MHz to 500 MHz (16534A):	1.00 div

**Input R:** 1 Meg Ohm +/-1%  
 50 Ohms +/-1%

\* = Specifications valid within +/-10 degrees C of self-calibration temperature

(1) Specification applies at the maximum sample rate. At lower rates, specification should be +/- (0.005% x delta t) + (2 x 10e-6 x delay setting) + (0.15 x sample interval) for bandwidth limited signals (tr = 1.4 x sample interval). Sample interval is defined as  $\frac{1}{\text{sample rate}}$

## Environmental Characteristics



### Probes

Maximum Input Voltage	1 Meg Ohm:	+/- 250V
	50 Ohms	5Vrms

### Operating Environment

Temperature	Instrument, 20 °C to 50 °C (+68 °F to 122 °F). Probe lead sets and cables, 0 °C to 65 °C (32 °F to 149 °F).
Humidity	Instrument, probe lead sets, and cables, up to 95% relative humidity at +40 °C (+122 °F).
Altitude	To 4600 m (15,000 ft).
Vibration	Operating: Random vibration 5 to 500 Hz, 10 minutes per axis, approximately 0.3 g(rms). Non-operating: Random vibration 5 to 500 Hz, 10 minutes per axis, approximately 2.41 g (rms); and swept sine resonant search, 5 to 500 Hz, 0.75 g (0-peak), 5 minute resonant dwell at 4 resonances per axis. Operating power supplied by mainframe. Indoor use only. Pollution Degree 2.

---

## Recommended Test Equipment

---

### Equipment Required

Equipment	Critical Specifications	Recommended Agilent Model/Part	Use*
Signal Generator	Frequency: 1 - 500 MHz at approx . 170 mV RMS Output Accuracy: $\pm 1$ dB 1 MHz time base accuracy 0.25 ppm	E4400B Option 1E5	P
DC Power Supply	Range: $-35.000$ to $+35.000$ Vdc, $\pm 1$ mV Resolution: 10 mV	3245A Option 002	P
Digital Multimeter	0.1 mV resolution Accuracy: better than 0.005% Resistance measurement: better than 0.25% accuracy	3458A	P
Power Meter/Sensor	1 - 500 MHz $\pm 3\%$ accuracy	E4418A/8482A	P
Power Splitter	Outputs differ by $<0.15$ dB	11667B	P
Blocking Capacitor	BNC (m)(f), 0.18 $\mu$ F, $\pm 200$ V	10240B	P
BNC Shorting Cap		1250-0074	P
Adapter	BNC (f)(f) (UG-914/U)	1250-0080	C
Adapter	BNC(f)-to-Dual Banana Plug	1251-2277	P
Adapter	Type N(m)-to-BNC(f)	1250-0780	P
BNC Tee	BNC (m)(f)(f)	1250-0781	P,C
Cable	Type N(m-to-m) 24-inch	11500B	P
Cable	50 $\Omega$ BNC (m-to-m) 48-inch	8120-1840	P, C
Cable (2)	50 $\Omega$ BNC (m-to-m) 9 inch	8120-1838	C

General Information  
**Recommended Test Equipment**





Preparing for Use

To inspect the module 2-2

To prepare the mainframe 2-3

To install the module 2-4

To configure the 16533A/34A module 2-4

To reconfigure a multicard module into single card modules 2-5

To turn on the system 2-6

To test the module 2-6

---

# Preparing For Use

This chapter gives you instructions for preparing the oscilloscope module for use.

## **Power Requirements**

All power supplies required for operating the oscilloscope are supplied through the backplane connector in the mainframe.

## **Operating Environment**

The operating environment is listed below. Note the noncondensing humidity limitation. Condensation within the instrument can cause poor operation or malfunction. Provide protection against internal condensation.

The oscilloscope module will operate at all specifications within the temperature and humidity range given below. However, reliability is enhanced when operating the module within the following ranges:

- **Temperature:** +20 °C to +35 °C (+68 °F to +95 °F)
- **Humidity:** 20% to 80% noncondensing

## **Storage**

Store or ship the oscilloscope in environments within the following limits:

- **Temperature:** –40 °C to + 75 °C
- **Humidity:** Up to 90% at 65 °C
- **Altitude:** Up to 15,300 meters (50,000 feet)

Protect the module from temperature extremes which cause condensation on the instrument.

---

## To inspect the module

### **1 Inspect the shipping container for damage.**

If the shipping container or cushioning material is damaged, keep them until you have checked the contents of the shipment and checked the instrument mechanically and electrically.

### **2 Check the supplied accessories.**

Accessories supplied with the module are listed in "Accessories" in chapter 1.

### **3 Inspect the product for physical damage.**

Check the module and the supplied accessories for obvious physical or mechanical defects. If you find any defects, contact your nearest Agilent Technologies Sales Office. Arrangements for repair or replacement are made, at Agilent Technologies' option, without waiting for a claim settlement.

---

## To prepare the mainframe

---

**CAUTION**

---

Turn off the mainframe power before removing, replacing, or installing the module.

---

**CAUTION**

---

Electrostatic discharge can damage electronic components. Use grounded wriststraps and mats when performing any service to this module.


- 1 Remove power from the instrument.
  - a Exit all logic analysis sessions. In the session manager, select Shutdown.
  - b At the query, select Power Down.
  - c When the "OK to power down" message appears, turn the instrument off.
  - d Disconnect the power cord.
  - e Disconnect any input or output connections.

- 2 Plan your module configuration.

If you are installing a one-card module, use any available slot in the mainframe.

If you are installing a multicard module, use adjacent slots in the mainframe.

- 3 Loosen the thumb screws.

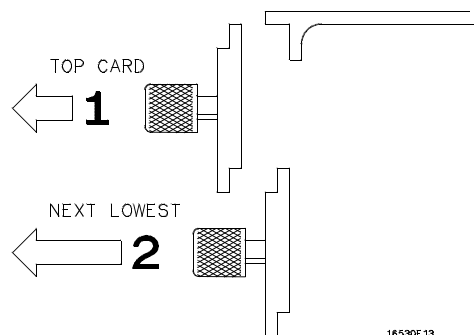

Cards or filler panels below the slots intended for installation do not have to be removed. Starting from the top, loosen the thumb screws on filler panels and cards that need to be moved.

- 4 Starting from the top, pull the cards and filler panels that need to be moved halfway out.

---

**CAUTION**

---

All multicard modules will be cabled together. Pull these cards out together to prevent damage to the cables and connectors.

- 5 Remove the cards and filler panels.

Remove the cards or filler panels that are in the slots intended for the module installation. Push all other cards into the card cage, but not completely in. This is to get them out of the way for installing the module.

Some modules for the Logic Analysis System require an operational accuracy calibration if you move them to a different slot. For calibration information, refer to the manuals for the individual modules.

---

## To install the module


The Agilent Technologies 16533A/34A oscilloscope module functions as either a master board or expander board. A single board 16533A/34A module provides 2 acquisition channels and a multichannel 16533A/34A module can provide up to 8 acquisition channels that operate from a single trigger.

The only requirements to configuring a multichannel 16533A or a multichannel 16534A module (more than one card) is connecting the cards together with the master/expander trigger cables. This is done after installing all cards and before applying power to the mainframe. In addition, a multichannel module should contain either all 16533A or 16534A cards.

---

## To configure the 16533/34A module


- 1 Slide the cards above the slot for the 16533A/34A module about halfway out of the mainframe.
- 2 Slide the 16533A/34A module approximately halfway into the mainframe. If a multichannel module is being configured, all 16533A/34A cards must be in adjacent slots.

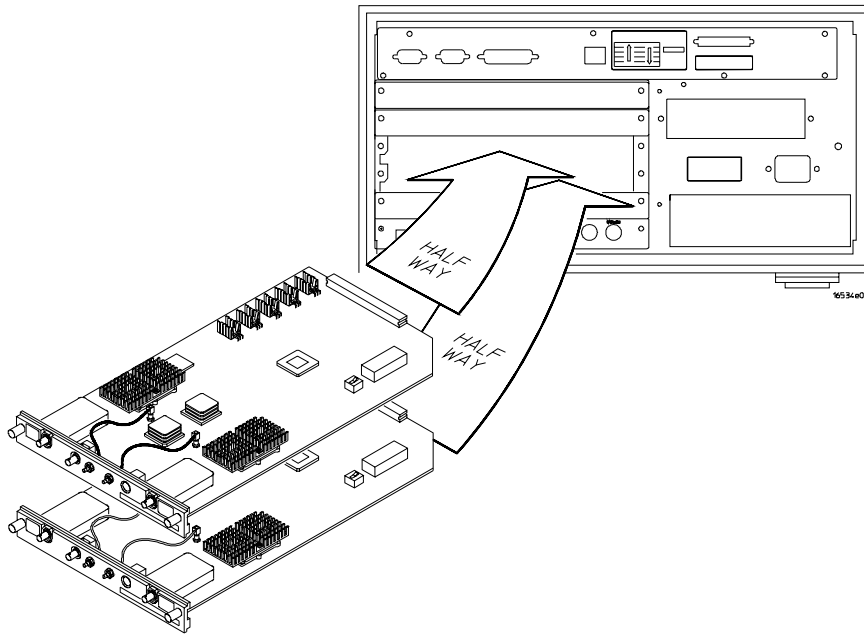

- 3 Position all cards and filler panels so that the endplates overlap.

**To reconfigure a multcard module into single card modules**


- 4 Seat the cards and tighten the thumbscrews. **DO NOT** use a Torx screwdriver to tighten the thumbscrews.

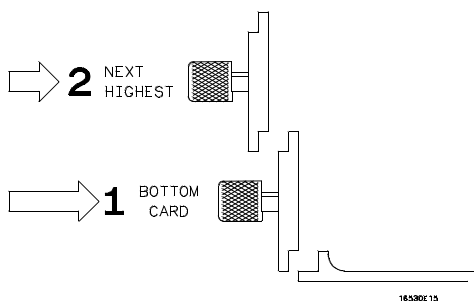

**WARNING**

For correct air circulation, filler panels must be installed in all unused card slots. Correct air circulation keeps the instrument from overheating. Keep any extra filler panels for future use.

- 5 To configure a multcard module, use the master/expander trigger cable included with the accessory kit of each 16533A/34A card. Starting with the top-most 16533A/34A card, connect the ECL EXT TRIG OUT to the ECL EXT TRIG IN of the card immediately below. Repeat for all cards in the module.

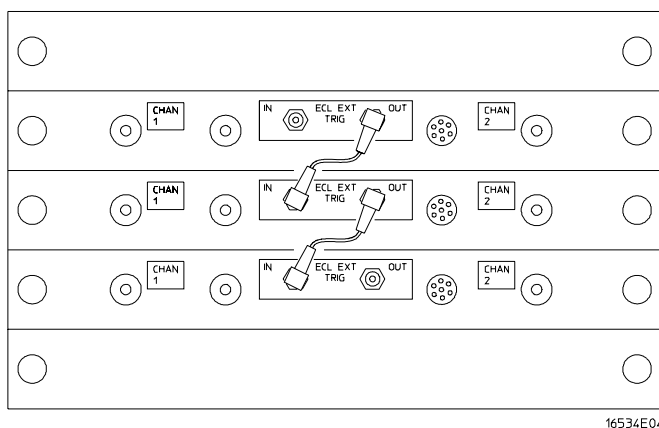

16534E04

**To reconfigure a multcard module into single card modules**

To reconfigure a multcard 16533A/34A module into single board modules, first remove power from the Agilent Technologies 16700-series mainframe. Remove all master/expander trigger cables from the rear panel of each 16533A/34A card in the module. Remove and reinstall each 16533A/34A card as desired and reapply power to the mainframe.


Performing an operational accuracy calibration on each reconfigured 16533A/34A card is recommended. Refer to Chapter 4 Calibrating and Adjusting.

---

## To turn on the system

- 1 Connect the power cable to the mainframe.
- 2 Turn on the power switch.

When you turn on the power switch, the oscilloscope performs power-up tests that check mainframe circuitry. After the power-up tests are complete, the screen will look similar to the sample screen below.

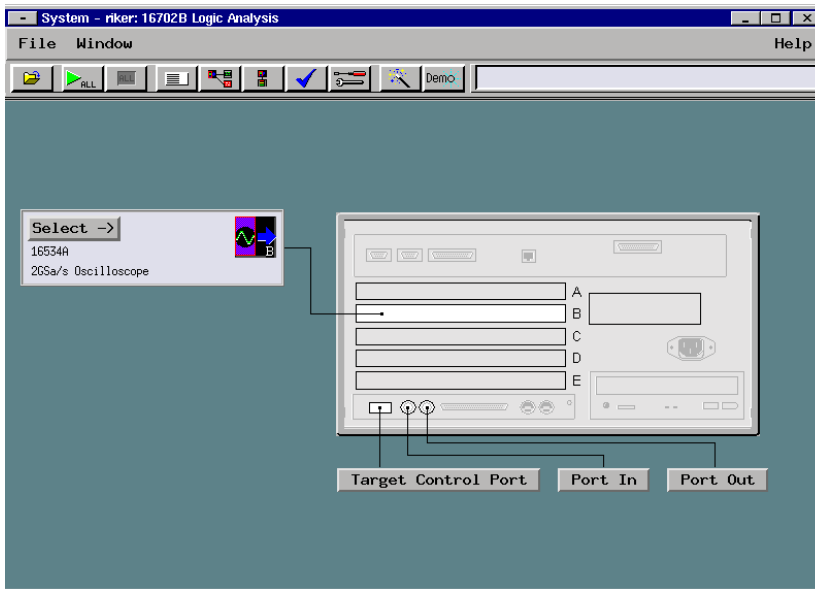

---

## To test the module

- If you require a test to initially accept the operation, perform the self tests in chapter 3.
- If you need to deskew the channel-to-channel variations, go to chapter 4, "Calibrating and Adjusting."
- If you require a test to verify the specifications, start at the beginning of chapter 3, "Testing Performance."
- If the module does not operate correctly, go to the beginning of chapter 5, "Troubleshooting."

To Perform the Self-tests 3-3  
Perform the power-up tests 3-3  
Perform the self-tests 3-4  
To test the input resistance 3-5  
Perform an operational accuracy calibration 3-9  
To test the voltage measurement accuracy 3-9  
To test the offset accuracy 3-16  
To test the bandwidth (16533A only) 3-24  
To test the bandwidth (16534A only) 3-31  
To test the time measurement accuracy 3-38  
To test the trigger sensitivity (16533A) 3-46  
To test the trigger sensitivity (16534A) 3-53  
Performance Test Record 3-60

---

# Testing Performance

This chapter tells you how to test the performance of the oscilloscope against the specifications listed in chapter 1. To ensure the oscilloscope is operating as specified, you perform software tests (self-tests) and manual performance tests on the oscilloscope. The oscilloscope is considered performance-verified if all of the software tests and manual performance tests have passed. The procedures in this chapter indicate what constitutes a "Pass" status for each of the tests. The procedures in this chapter are for both the Agilent Technologies 16533A and 16534A.

## **Test Strategy**

For a complete test, start at the beginning with the software tests and continue through to the end of the chapter. For an individual test, follow the procedure in the test.

The performance verification procedures starting on page 3–6 are each shown from power-up. To exactly duplicate the set-ups in the tests, save the power-up configuration to a file on a disk, then load that file at the start of each test.

If a test fails, check the test equipment set-up, check the connections, and verify adequate grounding.

## **Test Strategy for a Multicard Module**

A multicard 16533A/34A module must be separated into single card modules for all tests in this chapter. After testing the performance of each single card module, the module can then be reconfigured as a multicard module. At this point the 16533A/34A multicard module is ready for use.

## **Test Interval**

Test the performance of the oscilloscope against specifications (full calibration) at two-year intervals or if it is replaced or repaired.

## **Performance Test Record**

A performance test record for recording the results of each procedure is located at the end of this chapter. Use the performance test record to gauge the performance of the oscilloscope over time.

## **Test Equipment**

Each procedure lists the recommended test equipment. You can use equipment that satisfies the specifications given. However, the procedures are based on using the recommended model or part number. Before testing the performance of the oscilloscope, warm-up the instrument and the test equipment for 30 minutes.



---

## To Perform the Self-tests

There are two types of self-tests, self-tests that automatically run at power-up, and self-tests that you select on screen. The self-tests verify the correct operation of the logic analysis system. Self tests can be performed all at once or one at a time. While testing performance of the logic analysis system, run the self-tests all at once.

---

## Perform the power-up tests

The logic analysis system automatically performs power-up tests when you apply power to the instrument. Any errors are reported in the boot dialogue. Serious errors will interrupt the boot process.

The power-up tests are designed to complement the instrument on-line Self-Tests. Tests that are performed during power-up are not repeated in the Self Tests.

The monitor, keyboard, and mouse must be connected to the mainframe to observe the results of the power-up tests. (The 16702A does not require a monitor or keyboard. The 16702B does not require a monitor, mouse, or keyboard.)

**1 Disconnect all inputs and exit all logic analysis sessions.**

In the session Manager, select Shutdown. In the window, select Powerdown.

**2 When the "OK to power down" message appear, turn off the power switch.**

**3 After a few seconds, turn the power switch back on. Observe the boot dialogue for the following:**

- ensure all of the installed memory is reconginized
- any error messages
- interrupt of the boot process with or without error messages

A complete transcript of the boot dialogue is in the *Agilent Technologies 16700-Series Logic Analysis System Service Guide*, Chapter 8, "Theory of Operation."

**4 During initialization, check for any failures.**

If an error or interrupt occurs, refer to the *Agilent Technologies 16700-Series Logic Anaylisis System Service Guide*, Chapter 5, "Troubleshooting."

## Perform the self-tests

The self-tests verify the correct operation of the logic analysis system and the installed 16533/34 module. Self-tests can be performed all at one or one at a time. While testing the performance of the logic analysis system, run the self-tests all at once.

### **1 Launch the Self-Tests**

- a** In the System window, select System Admin.
- b** Under the Admin tab, select Self-Test...
- c** In the query pop-up, select Yes to exit the current session.

The Self-Test closes down the current session because the test algorithms leave the system in an unknown state. Re-launching a session at the end of the tests will ensure the system is properly initialized.

### **2 In the Self-Test window, select Test All.**

When the tests are finished, the Status will change to TEST passed or TEST failed. You can find detailed information about the test results in the Status Message field of the Self-Test window.

The System CPU Board test returns Untested because the CPU test require user action. To test the CPU Board, select CPU Board, then select each test individually.

### **3 Select Quit to exit the Test menu.**

### **4 In the Session Manager, select Start Session to re-launch a logic analysis session.**

---

## To test the input resistance

Testing the input resistance verifies the performance of the following specification:

- **Input resistance**

This test checks the input resistance at the 50  $\Omega$  and 1 M $\Omega$  settings in the Coupling field.

---

### Equipment Required

---

Equipment	Critical Specifications	Recommended Agilent Model/Part
Digital Multimeter	Measure resistance (4-wire) better than 0.25% accuracy	3458A
Cables (2)	BNC (m)(m) 48-inch	8120-1840
Adapter	BNC Tee (m)(f)(f)	1250-0781
Adapters (2)	BNC (f) to Dual Banana Plug	1251-2277


---

### Set up the equipment

- 1 Turn on the equipment required and the logic analysis system mainframe with the oscilloscope module to be tested. Let them warm up for 30 minutes if you have not already done so.
- 2 Set up the multimeter to make a 4-wire resistance measurement.


## Set up the oscilloscope

- 1 Set up the oscilloscope.
  - a In the Logic Analysis System window, select the module icon, then select Setup/Display. The oscilloscope Setup/Display window opens.
  - b Select the Channel 2 On field, and the field will toggle to Off.

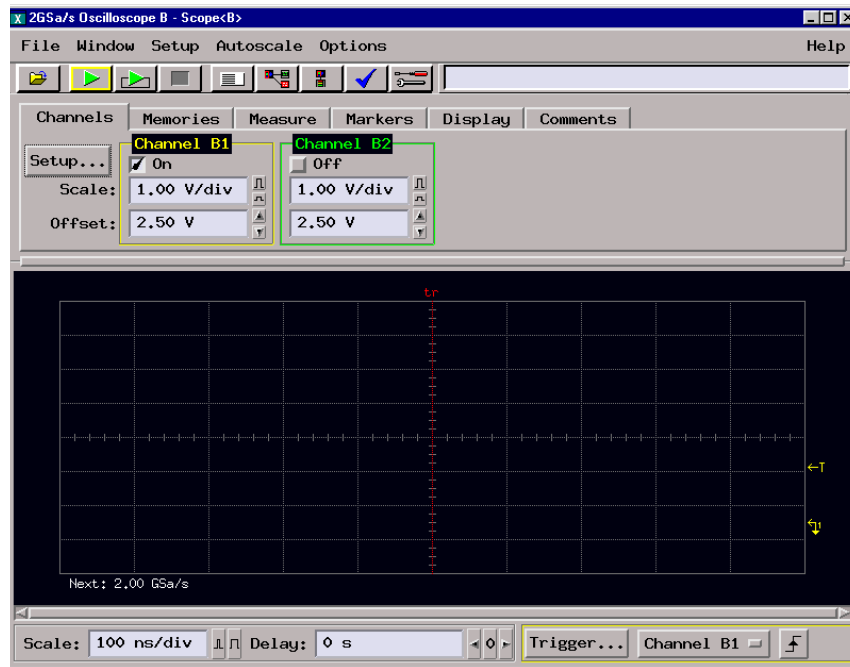

- 2 Set up the Channel.
  - a Under the Channel tab, select Setup. The Channel Setup window opens.
  - b Select the Probe field, then enter 1.000:1.
  - c Select Input Z/Coupling: 50 Ohm/DC.
  - d Select the Scale field, then enter 20 mV/div.

- e Select the Offset field, then enter 0 V.

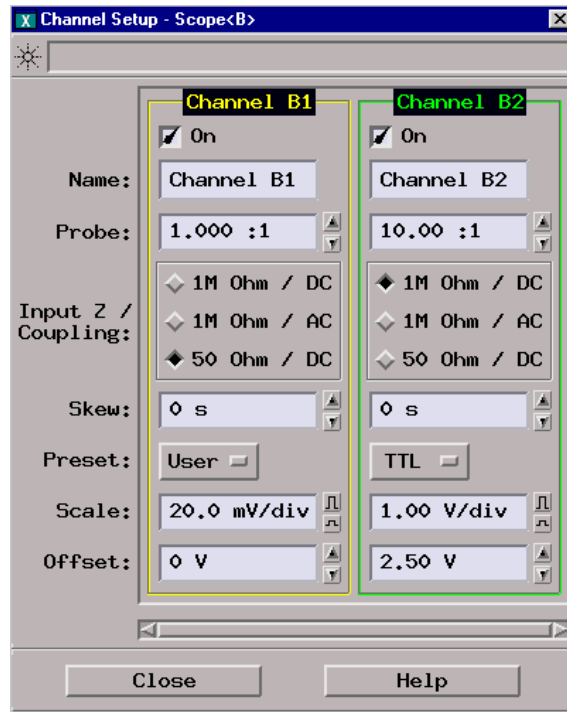

Leave the channel Setup window open. You will be changing settings in this window as you complete this test.

- 3 Set up the Trigger.
  - a At the bottom of the display, select Trigger.
  - b In the trigger Setup window, select Mode Immediate.




- c Select Close to close the Trigger Setup window.

---

## Connect the oscilloscope

Using the BNC-to-banana adapters, connect one end of each BNC cable to the 4-wire resistance connections on the multimeter, and connect the free ends of the cables to the BNC Tee. Connect the male end of the BNC tee to the channel 1 input of the oscilloscope module.

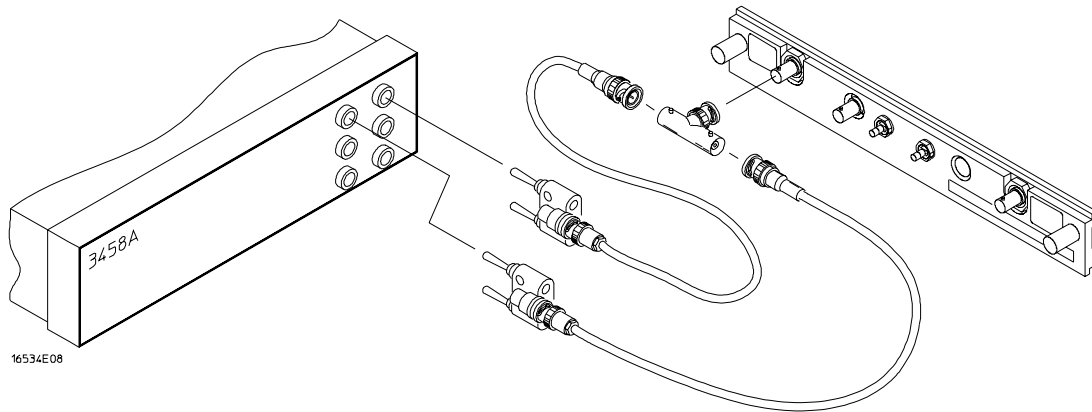

---

## Acquire the data

- 1 Select the Run icon. The clicking of attenuator relays should be audible. Verify resistance readings on the digital multimeter of  $50\ \Omega \pm 0.5\ \Omega$  (49.5 to 50.5  $\Omega$ ). Record the reading in the performance test record.
- 2 In the Channel Setup window change the Channel 1 Input Z/Coupling field to 1M $\Omega$ /DC.
- 3 Select Run. Verify resistance readings on the digital multimeter of  $1\ \text{M}\Omega \pm 10\ \text{k}\Omega$  (0.990 to 1.010  $\text{M}\Omega$ ). Record the reading in the performance test record.
- 4 In the Channel Setup window, change the Channel 1 Input Z/Coupling field to 50  $\Omega$ /DC and V/div to 200 mV/div. Repeat steps 1 through 3.
- 5 In the Channel Setup window, change the Channel 1 Input Z/Coupling field to 50  $\Omega$ /DC and V/div to 1 V/div. Repeat steps 1 through 3.
- 6 In the Channel Setup window, change the Channel 1 Input Z/Coupling field to 50  $\Omega$ /DC and V/div to 5 V/div. Repeat steps 1 through 3.
- 7 Connect the male end of the BNC tee to the channel 2 input of the oscilloscope module.
- 8 Repeat from "Set up the oscilloscope" for channel 2, replacing channel 1 with channel 2 where applicable.

### See Also

If a reading is not within limits, then the attenuator for the out-of-bounds channel should be replaced (see chapter 6).

---

## Perform an operational accuracy calibration

At this point, an operational accuracy calibration should be performed. Follow the procedure in chapter 4, "To calibrate the oscilloscope."

Record the results in the performance test record.

---

## To test the voltage measurement accuracy

Testing the voltage measurement accuracy verifies the performance of the following specification:

- Voltage measurement accuracy

This test verifies the DC voltage measurement accuracy of the instrument, using a dual cursor measurement that nullifies offset error.

---

### Equipment Required

Equipment	Critical Specifications	Recommended Agilent Model/Part
DC Power Supply	-35.000 Vdc to +35.000 Vdc, 0.1 mV resolution	3245A Option 002
Digital Multimeter	Better than 0.1% accuracy	3458A
Cable	BNC (m)(m) 48-inch	8120-1840
Adapter (cable to power supply)	BNC (f) to Dual Banana Plug	1251-2277
Adapter	BNC tee (m)(f)(f)	1250-0781
Blocking Capacitor	BNC (m)(f) 0.18 $\mu$ F, $\pm$ 200 V	10240B
BNC Shorting Cap		1250-0074

---


## Set up the equipment

Turn on the equipment required and the logic analysis system mainframe with the oscilloscope module to be tested. Let them warm up for 30 minutes if you have not already done so.

---

## Set up the oscilloscope


- 1 Set up the oscilloscope.
  - a In the Logic Analysis System window, select the module icon, then select Setup/Display. The oscilloscope Setup/Display window opens..
  - b Select the Channel 2 On field, and the field will toggle to off.
  - c At the bottom of the Setup/Display window, select the Scale field, then enter 2.00 ms/div.

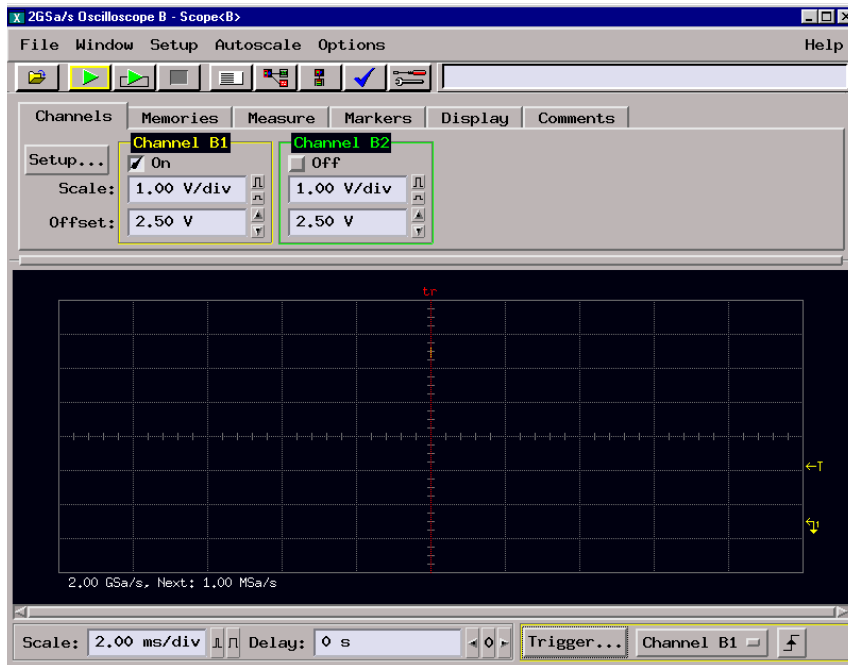

- 2 Set up the Channel.
  - a Under the Channels tab, select Setup. The Channel Setup window opens.
  - b Select the Probe field, then enter 1.000:1.
  - c Select Input Z/Coupling: 1M Ohm/DC.




**CAUTION** Set the Channel Input Z/Coupling field to 1M Ohm/DC or damage to the equipment will result.

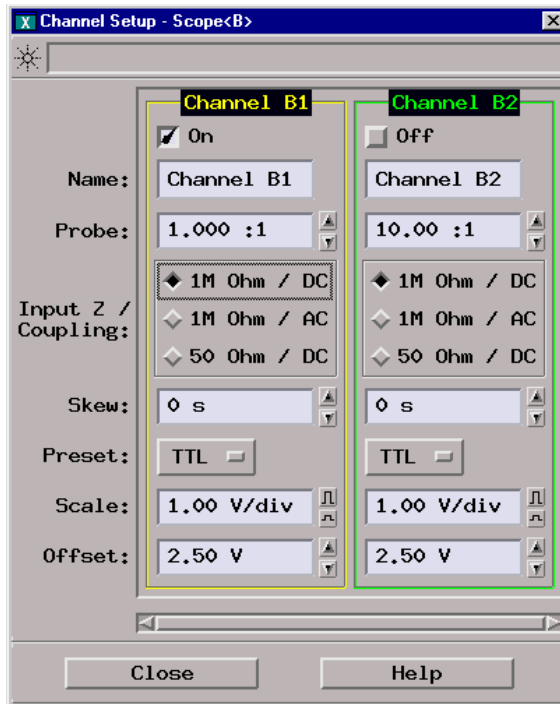


Leave the channel Setup window open. You will be changing settings in this window as you complete this test.


- 3 Set up the Display.
  - a In the oscilloscope Setup/Display window, select the Display tab.
  - b Select Waveform Mode Average, and set # Avgs: 16.

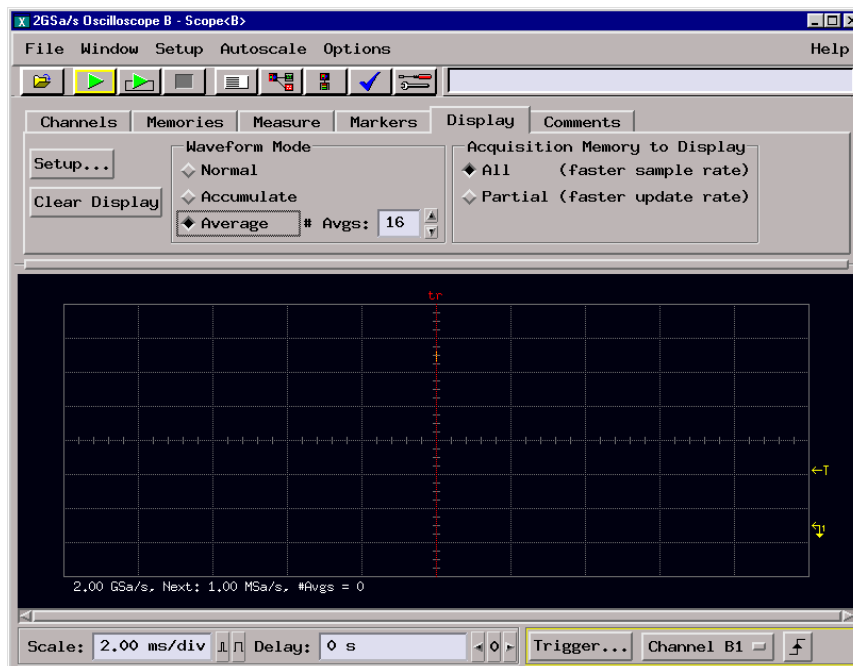

- 4 Set up the Trigger.
  - a At the bottom of the display, select Trigger.
  - b In the trigger Setup window, select Mode Immediate.

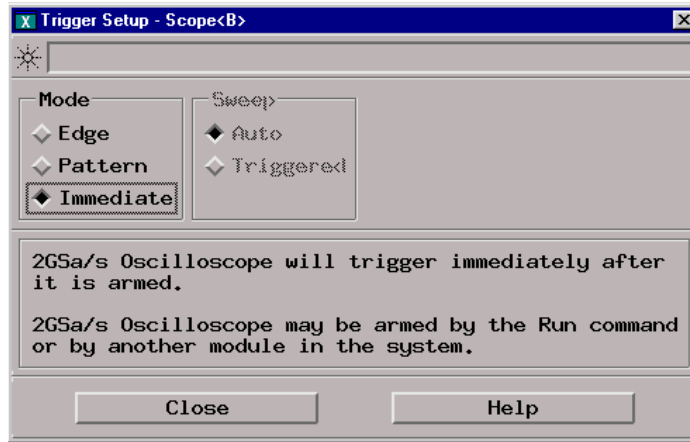


- c Select Close to close the Trigger Setup window.
- 5 Set up Markers.
  - a In the oscilloscope Setup/Display window, select the Markers tab.
  - b Under the Markers tab, select Setup. The Markers Setup window opens.
  - c In the Marker Setup window, select the V1 button to turn on marker V1. Select the channel assignment for V1, and select Channel 1.
  - d In the Marker Setup window, select the V2 button to turn on marker V2. Select the channel assignment for V2, and select Channel 1.

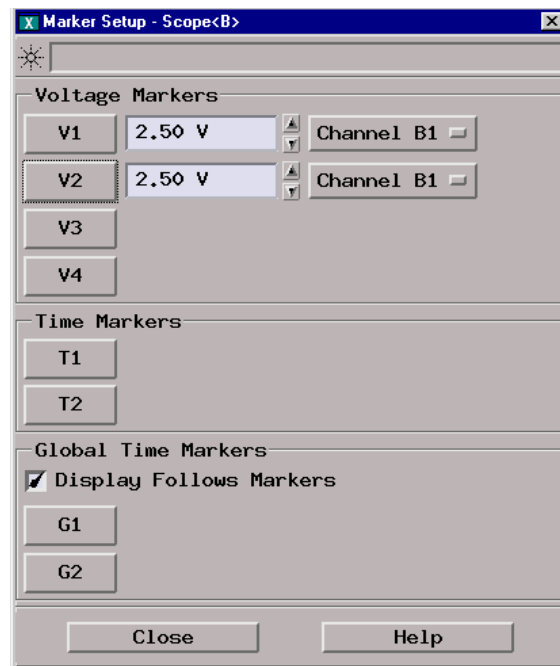

- e Select Close to close the Marker Setup window.

## Connect the oscilloscope

- 1 Using a BNC-to-banana adapter, connect one end of the cable to the power supply. Connect the BNC tee, the blocking capacitor, and the shorting endcap to the other end of the cable.
- 2 Monitor the power supply output with the Digital Multimeter.

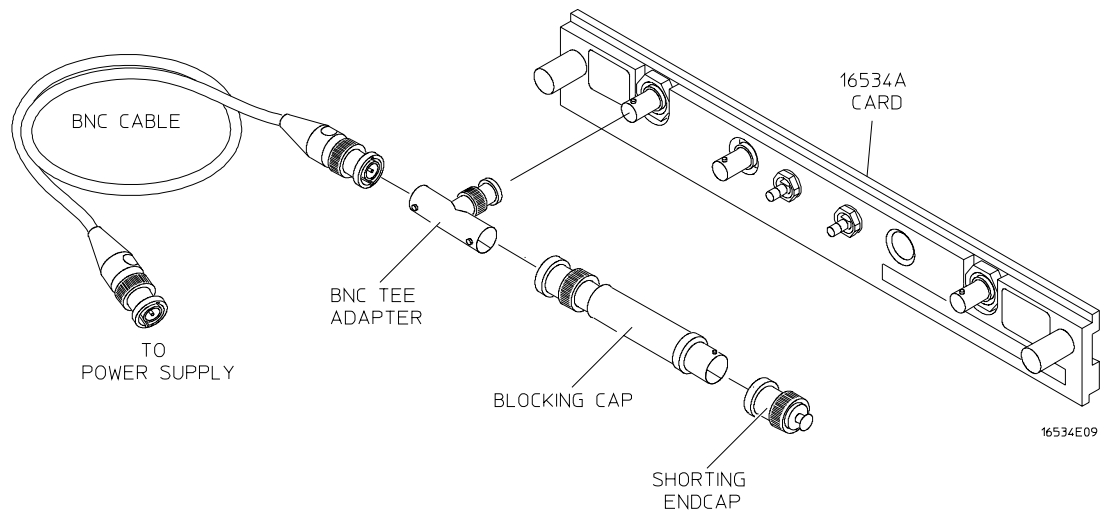

## Acquire the data

Use the following table for steps 1 through 4.


Oscilloscope Settings			Voltage Readings		
Scale	Offset	Supply	Tolerance*	Upper Limit	Lower Limit
5 V/div	-17.5 V	-35.0 V	+/-660 mV	-34.340 V	-35.660 V
1 V/div	-3.5 V	-7.0 V	+/-132 mV	-6.868 V	-7.132 V
200 mV/div	-700.0 mV	-1.4 V	+/-26.4 mV	-1.374 V	-1.426 V
40 mV/div	-140.0 mV	-280 mV	+/-5.28 mV	-274.8 mV	-285.2 mV
40 mV/div	140.0 mV	280 mV	+/-5.28mV	285.2 mV	274.8 mV
200 mV/div	700.0 mV	1.4 V	+/-26.4 mV	1.426 V	1.374 V
1 V/div	3.5 V	7.0 V	+/-132 mv	7.132 V	6.868 V
5 V/div	17.5 V	35.0 V	+/-660 mV	35.660 V	34.340 V

\*Because a dual cursor measurement is taken, offset error is nullified.

- 1 Set up the oscilloscope according to the table above.
  - a In the Channel Setup window, select the Scale field, then enter the V/div values shown on the first line of the table.

Testing Performance  
To test the voltage measurement accuracy

- b In the Channel Setup window, select the Offset field, then enter the offset value shown on the first line of the table.

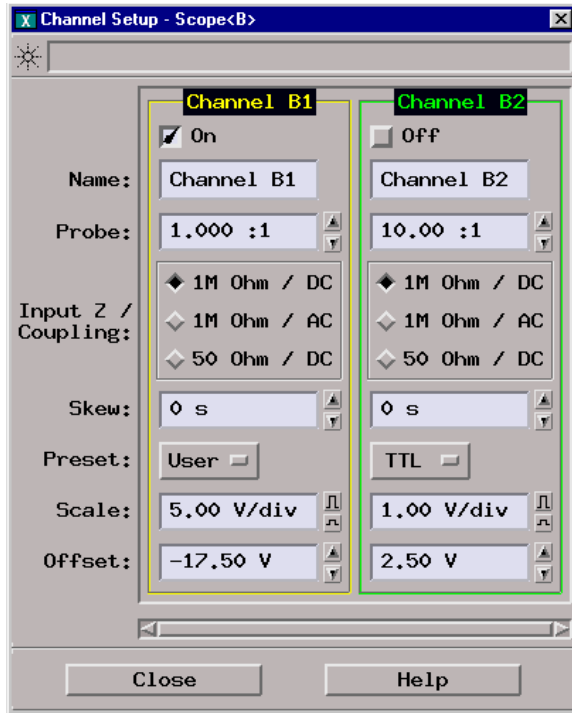

- 2 Acquire the zero input voltage.
- a Disconnect the power supply cable from the oscilloscope channel input.
  - b Select Run-Repetitive. Wait for averaging to complete, then select Stop.
  - c Using the mouse, position the cursor over the V1 marker. Then click and drag the V1 marker until it is over the oscilloscope trace on the display.



- 3 Acquire the measured voltage.
  - a Connect the power supply to the channel input. Set the power supply voltage according to the first line of the table.
  - b Move the mouse cursor over the waveform display and do a right mouse click. At the popup window select Clear Display.
  - c Select Run-Repetitive. Wait for averaging to complete, then select Stop.
  - d Using the mouse, position the cursor over the V2 marker. Then click and drag the V2 marker until it is over the oscilloscope trace on the display.
  - e In the oscilloscope Setup/Display window under the Markers tab, read the V2 - V1 voltage. The value should be between the minimum and maximum values listed in the table. Record the value in the performance test record.



- f Again move the mouse cursor over the waveform display and do a right mouse click. At the popup window select Clear Display.
- 4 Repeat steps 1 through 3 for the second line of the table, then for the rest of the lines of the table for channel 1.
- 5 Repeat from "Set up the oscilloscope" for channel 2, replacing channel 1 with channel 2 where applicable.

---

## To test the offset accuracy

Testing the offset accuracy verifies the performance of the following specification:

- Offset accuracy

---

### Equipment Required

Equipment	Critical Specifications	Recommended Agilent Model/Part
DC Power Supply	-35.000 to +35.000 Vdc, $\pm 1$ mV resolution	3245A Option 002
Digital Multimeter	Better than 0.1% accuracy	3458A
Cable	BNC (m)(m) 48-inch	8120-1840
Adapter (cable to power supply)	BNC (f) to Dual Banana Plug	1251-2277
Adapter	BNC tee (m)(f)(f)	1250-0781
Blocking Capacitor	BNC (m)(f) 0.18 $\mu$ F, $\pm 200$ V	10240B
BNC Shorting Cap		1250-0074


---

## Set up the equipment

Turn on the equipment required and the logic analysis system mainframe with the oscilloscope module to be tested. Let them warm up for 30 minutes if you have not already done so.

## Set up the oscilloscope


- 1 Set up the oscilloscope.
  - a In the Logic Analysis System window select the module icon, then select Setup/Display. The oscilloscope Setup/Display window opens.
  - b Select the Channel 2 On field, and the field will toggle to Off.
  - c At the bottom of the Setup/Display window, select the Scale field, then enter 2.00 ms/div.

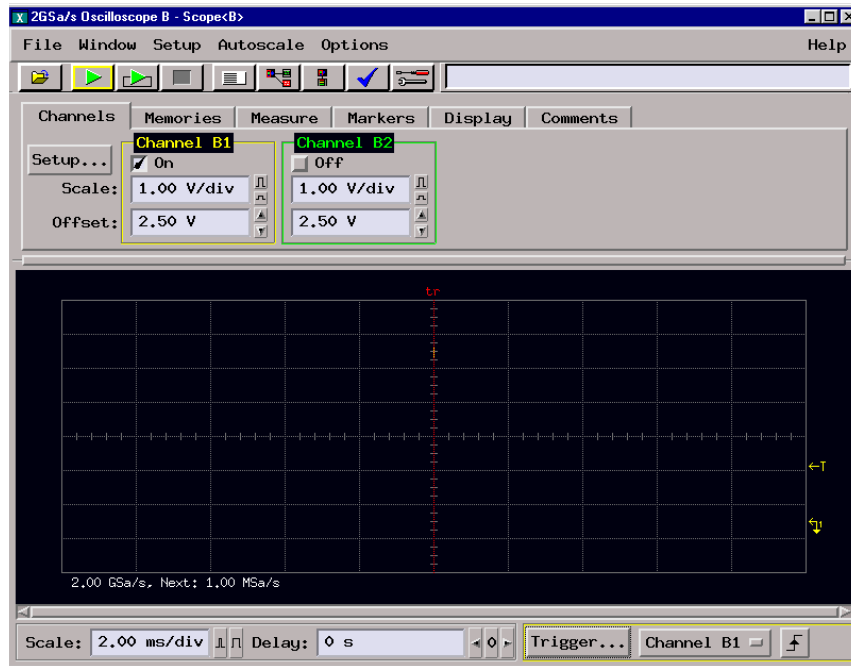

- 2 Set up the Channel.
  - a Under the Channels tab, select Setup. The Channel Setup window opens.
  - b Select the Probe field, then enter 1.000:1.
  - c Select Input Z/Coupling: 1M Ohm/DC.

**CAUTION**


Set the channel Input Z/Coupling field to 1M Ohm/DC or damage to the equipment will result.

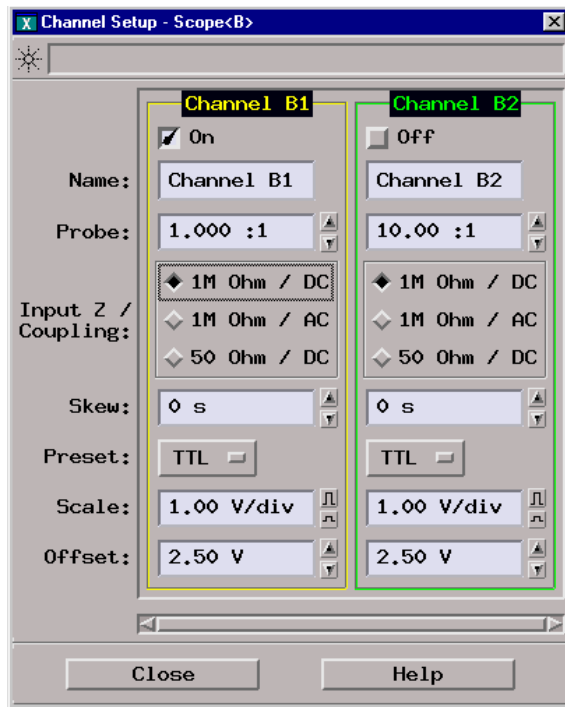

Leave the Channel Setup window open. You will be changing setting in this window as you complete this test.

**3** Set up the Display.

- a** In the oscilloscope Setup/Display window, select the Display tab.
- b** Select Waveform Mode Average, and set # Avgs:16.

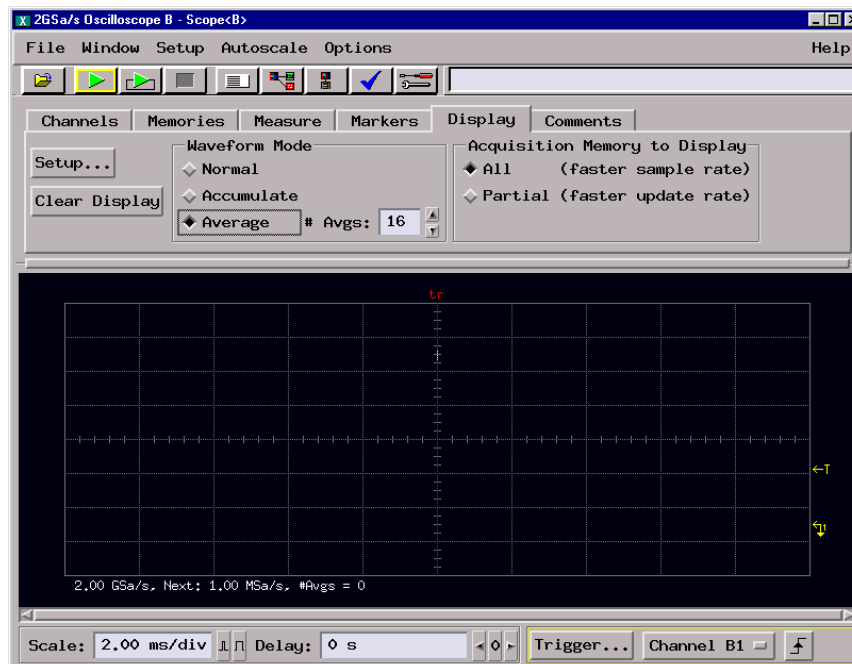



4 Set up Trigger.


- a At the bottom of the display, select Trigger.
- b In the Trigger Setup window, select Mode Immediate.



- c Select Close to close the Trigger Setup window.

5 Set up Markers.


- a In the oscilloscope Setup/Display window, select the Markers tab.
- b Under the Markers tab, select Setup. The Markers Setup window opens.
- c In the Marker Setup Window select the V1 button to turn on marker V1. Select the channel assignment for V1, and select Channel 1.

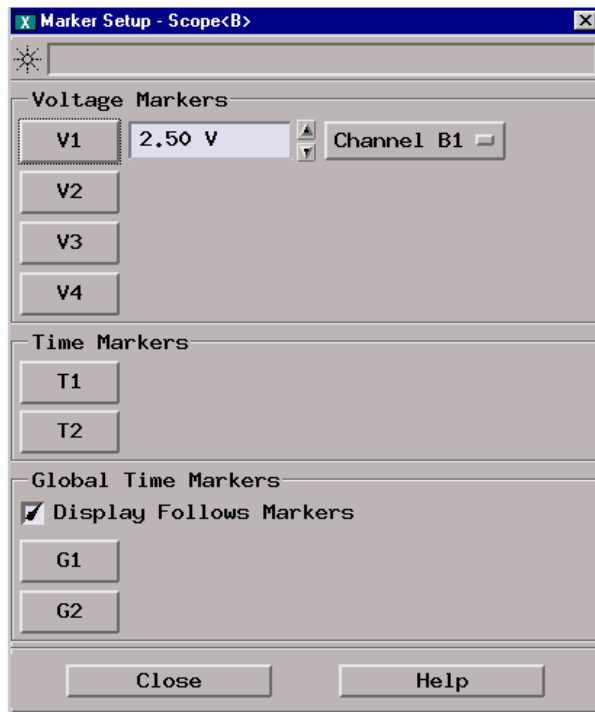

- d Select Close to close the Marker Setup window.

## Connect the oscilloscope

- 1 Using a BNC-to-banana adapter, connect one end of the cable to the power supply. Connect the BNC tee, the blocking capacitor, and the shorting endcap to the other end of the cable.
- 2 Monitor the power supply output with the Digital Multimeter.

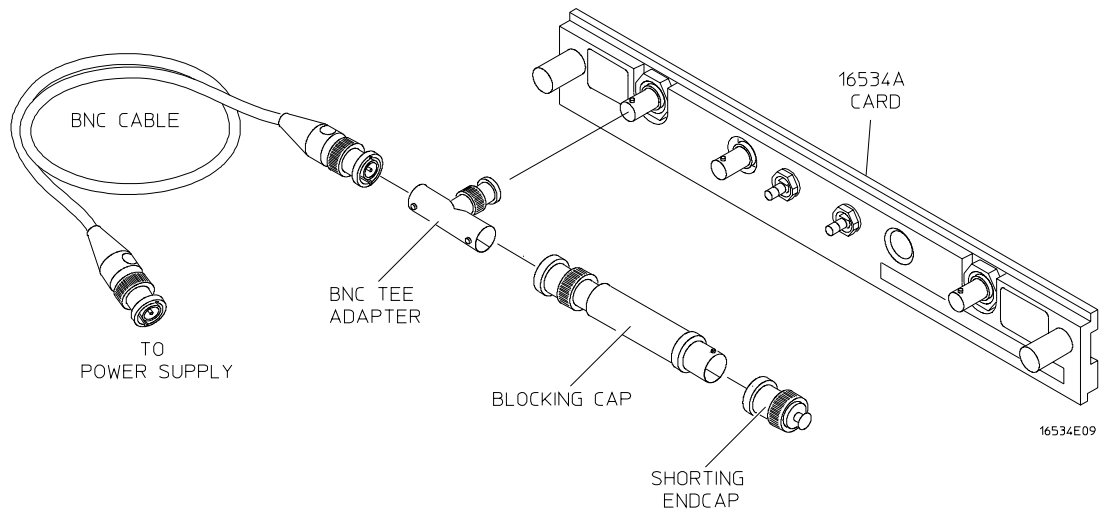


## Acquire the zero input data

Use the following table for steps 1 through 4.

Oscilloscope Settings		Voltage Readings		
Scale	Offset	Tolerance	Upper Limit	Lower Limit
5 V/div	0 V	+/-800 mV	800.0 mV	-800.0 mV
1 V/div	0 V	+/-160 mV	160.0 mV	-160.0 mV
200 mV/div	0 V	+/-32.0 mV	32.0 mV	-32.0 mV
40 mV/div	0 V	+/-6.4 mV	6.4 mV	-6.4 mV

- 1 Disconnect the power supply cable from the oscilloscope channel input.
- 2 Set up the oscilloscope according to the table above.
  - a In the Channel Setup window, select the Scale field, then enter the V/div values shown on the first line of the table.

- b In the Channel Setup window, select the Offset field, then enter 0 V.

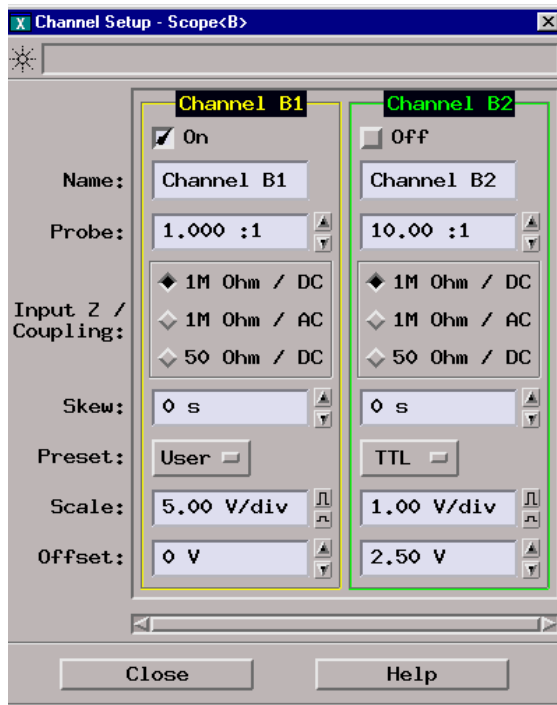

- 3 Acquire the zero input voltage.
- Select Run-Repetitive. Wait for averaging to complete, then select Stop.
  - Using the mouse, position the cursor over the V1 marker. Then click and drag the V1 marker until it is over the oscilloscope trace on the display.
  - In the oscilloscope Setup/Display window under the Markers tab, read the V1 voltage. The value should be between the minimum and maximum values listed in the table. Record the value in the performance test record.





- d In the oscilloscope Setup/Display window under the Markers tab, read the V1 voltage. The value should be between the minimum and maximum values listed in the table. Record the value in the performance test record.



- e Move the mouse cursor over the waveform display and do a right mouse click. At the popup window select Clear Display.
- Repeat steps 1 through 3 for the second line of the table, then for the rest of the lines of the table for channel 1.
  - Repeat from "Set up the oscilloscope" for channel 2, replacing channel 1 with channel 2 where applicable.

---

## To test the bandwidth (16533A only)

Testing the bandwidth verifies the performance of the following specification:

- **Bandwidth**

This test verifies the bandwidth (dc coupled) of the instrument.

---

### Equipment Required

---

<b>Equipment</b>	<b>Critical Specifications</b>	<b>Recommended Agilent Model/Part</b>
Signal Generator	1 - 250 MHz at approx 170 mV rms	E4400B Option 1E5
Power Meter/Sensor	1 - 250 MHz $\pm$ 3% accuracy	E4418A/8482A
Power Splitter	Outputs differ by <0.15 dB	11667B
Cable	Type N (m)(m) 24-inch	11500B
Adapter	Type N (m) to BNC (f)	1250-0082


---

## Set up the equipment

Turn on the equipment required and the logic analysis system mainframe with the oscilloscope module to be tested. Let them warm up for 30 minutes if you have not already done so.


## Set up the oscilloscope

- 1 Set up the oscilloscope.
  - a In the Logic Analysis System window, select the module icon, then select Setup/Display. The oscilloscope Setup/Display window opens.
  - b Select the Channel 2 On field, and the field will toggle to Off.
  - c At the bottom of the Setup/Display window, select the Scale field, then enter 200 ns/div.

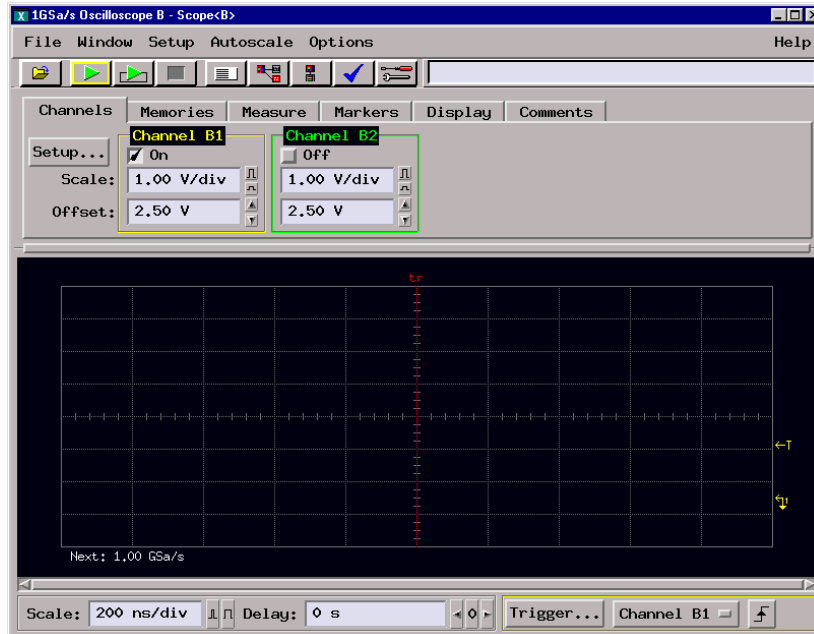

- 2 Set up the Channel.
  - a Under the Channels tab, select Setup. The Channel Setup window opens.
  - b Select the Probe field, then enter 1.000:1.
  - c Select Input Z/Coupling: 50 Ohm/DC.
  - d Select the Scale field, then enter 40 mV/div.


- e Select the Offset field, then enter 0 V.

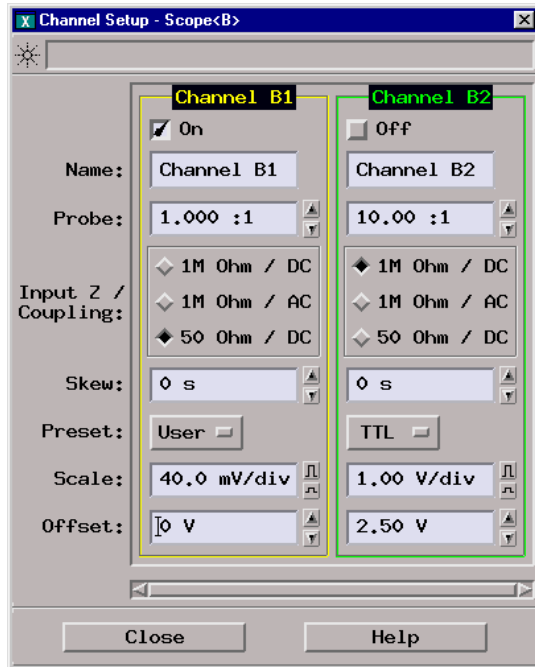

- f Select Close to close the Channel Setup window.

3 Set up the Display.

- a In the oscilloscope Setup/Display window, select the Display tab.  
b Select Waveform Mode Average, and set # Avgs: 32.

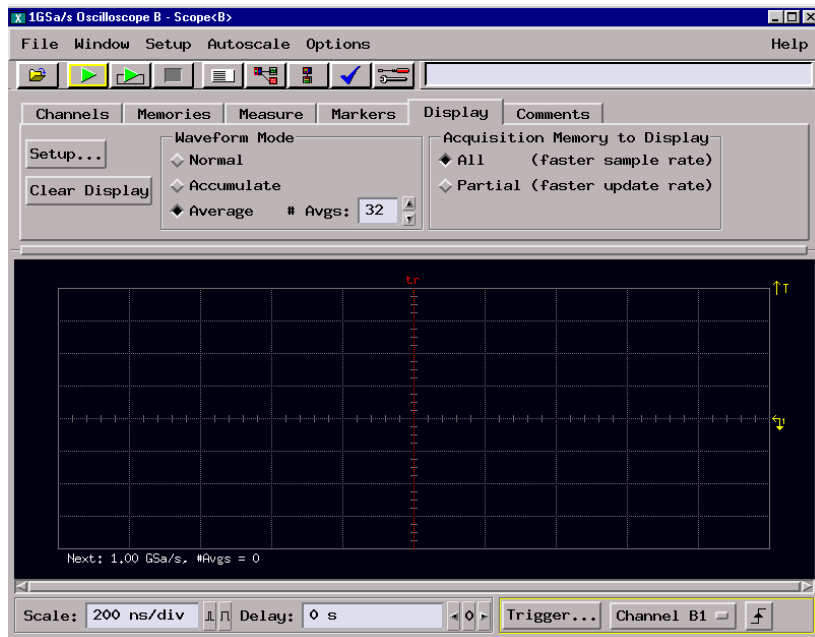


4 Set up the Trigger.


- a At the bottom of the display, select Trigger.  
b In the Trigger Setup window, select Mode Edge.



- c Select the Source field, then select Channel 1.
- d Select the Level field, then enter 0 V.

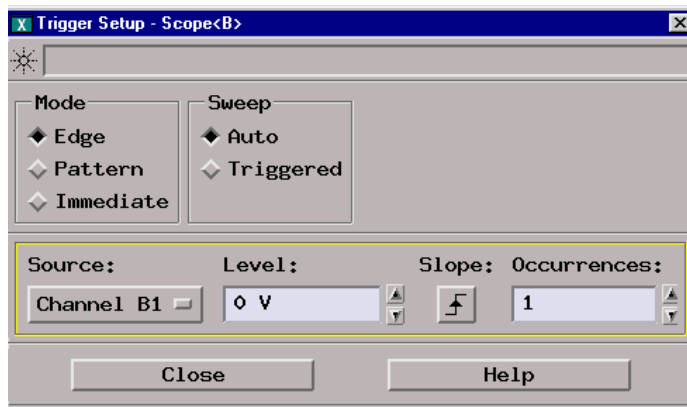

- e Select Close to close the Trigger Setup window.
- 5 Ensure the Markers are turned off.
- a In the oscilloscope Setup/Display window, select the Markers tab.
  - b Under the Markers tab, select Setup. The Markers Setup window opens.
  - c In the Marker Setup window, ensure all markers are disabled, as shown.

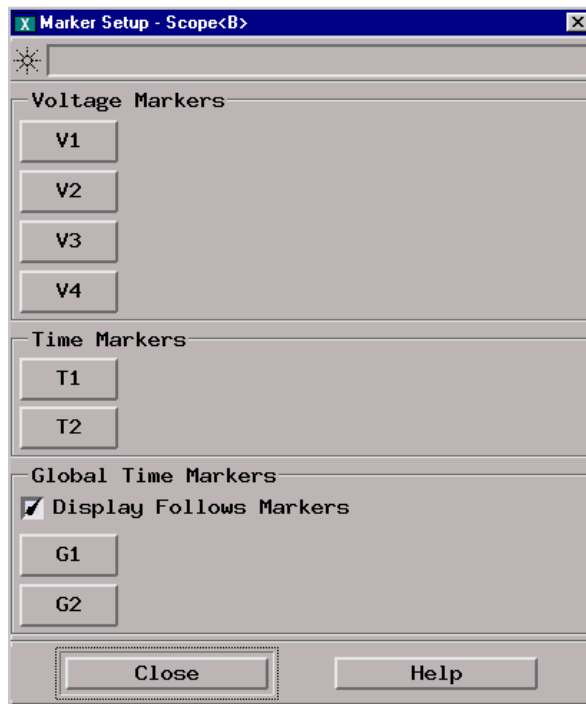


- d Select Close to close the Marker Setup window.

---

## Connect the oscilloscope

- 1 Using the N cable, connect the signal generator to the power splitter input. Connect the power sensor to one output of the power splitter.
- 2 Using the N-to-BNC adapter, connect the other power splitter output to the channel 1 input of the oscilloscope.

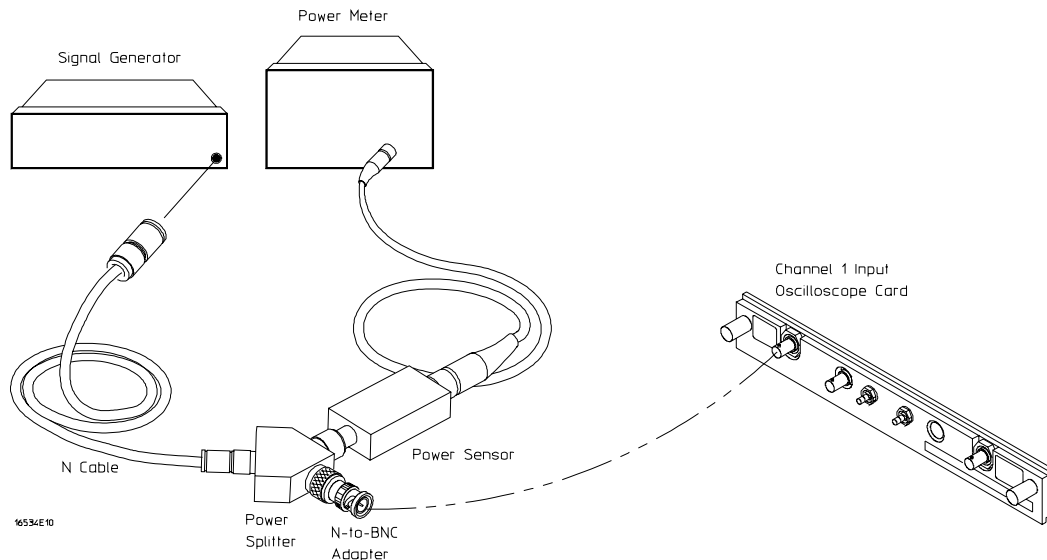


---

## Acquire the data


- 1 Obtain the 1 MHz response.
  - a Set the signal generator for 1 MHz at  $-2.4$  dBm.
  - b Select Run-Repetitive. The signal on the screen should be two cycles at six divisions amplitude. After averaging is complete select Stop.

- c In the oscilloscope Setup/Display window, select the measure tab. Note the voltage reading in the  $V_{p-p}$  field.

$V_{1\text{ MHz}} = \underline{\hspace{2cm}}$  mV.

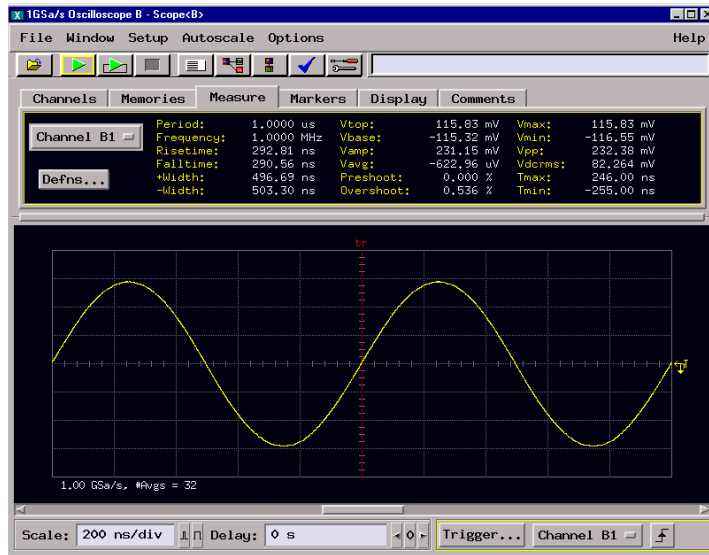

- 2 Set the signal generator for 250 MHz frequency.
  - a Set the power meter Cal Factor % to the 1 MHz value from the calibration chart on the power splitter. Press dB[REF] to set a 0 dB reference.
  - b Change the signal generator frequency to 250 MHz. Set the power meter Cal Factor % to the 250 MHz value from the chart.
  - c Adjust the signal generator amplitude for a power reading as close as possible to 0.0 dB[REL] and note the power reading. Reading =  $\underline{\hspace{2cm}}$  dB.
- 3 Obtain the 250 MHz response.
  - a At the bottom of the Setup/Display window, select the Scale field, then enter 2 ns/div.
  - b Select Run-Repetitive. After averaging is complete, select Stop.
  - c Note the voltage reading in the  $V_{p-p}$  field  $V_{250\text{ MHz}} = \underline{\hspace{2cm}}$  mV.

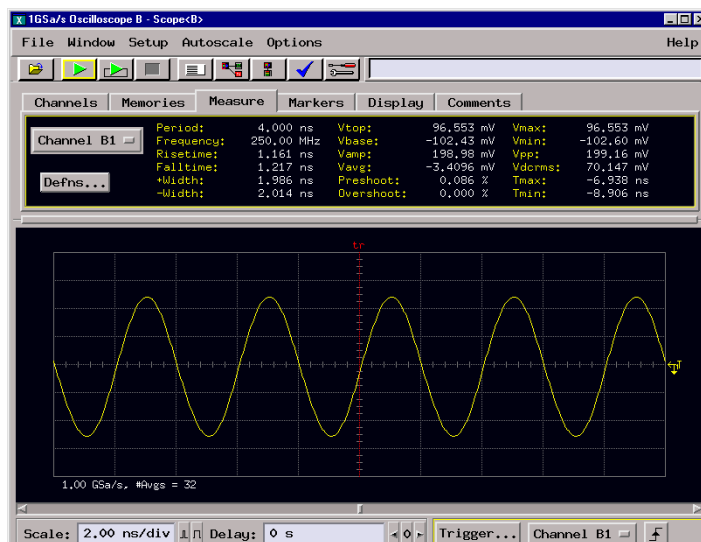

**4** Determine the oscilloscope response.

**a** Calculate the response using the formula:

$$response (dB) = 20 \log_{10} \frac{V_{250MHz}}{V_{1MHz}} = 20 \log_{10} (\text{_____}) = \text{_____} dB$$

**b** Correct the result from step 4a above with any differences in the power meter from step 2c. Observe signs. For example:

Result from step 4a = -1.34 dB

Power meter reading = -0.2 dB[REL]

then true response = (-1.34) - (-0.20) = -1.14 dB

(\_\_\_\_\_) - (\_\_\_\_\_) = \_\_\_\_\_ dB

**c** The result from step 4b should be  $\leq -3.0$  dB. Record the result in the performance test record.

**5** Remove the power splitter from the oscilloscope module channel 1 input and connect it to the channel 2 input.

**6** Repeat from "Set up the oscilloscope" for channel 2, replacing channel 1 with channel 2 where applicable.

**See Also**

Failure of the bandwidth test can be caused by a faulty attenuator or main assembly (see chapter 6).

---

## To test the bandwidth (16534A only)

Testing the bandwidth verifies the performance of the following specification:

- **Bandwidth**

This test verifies the bandwidth (dc coupled) of the instrument.

---

### Equipment Required

---

Equipment	Critical Specifications	Recommended Agilent Model/Part
Signal Generator	1 - 500 MHz at approx 170 mV rms	E4400B Option 1E5
Power Meter/Sensor	1 - 500 MHz $\pm$ 3% accuracy	E4418A/8482A
Power Splitter	Outputs differ by <0.15 dB	11667B
Cable	Type N (m)(m) 24-inch	11500B
Adapter	Type N (m) to BNC (f)	1250-0082


---

### Set up the equipment

Turn on the equipment required and the logic analysis system mainframe with the oscilloscope module to be tested. Let them warm up for 30 minutes if you have not already done so.


## Set up the oscilloscope

- 1 Set up the oscilloscope.
  - a In the Logic Analysis System window, select the module icon, then select Setup/Display. The oscilloscope Setup/Display window opens.
  - b Select the Channel 2 On field, and the field will toggle to Off.
  - c At the bottom of the Setup/Display window, select the Scale field, then enter 200 ns/div.

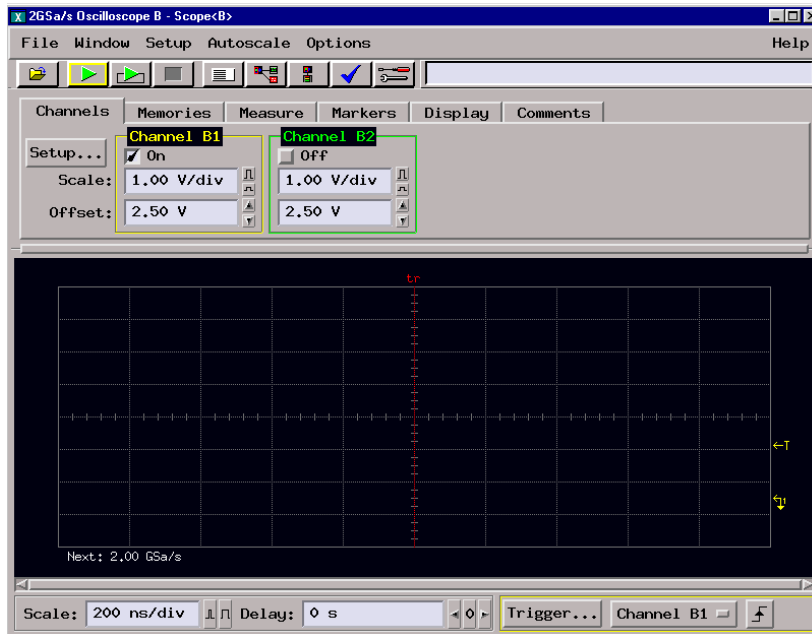


- 2 Set up the Channel.
  - a Under the Channels tab, select Setup. The Channel Setup window opens.
  - b Select the Probe field, then enter 1.000:1.
  - c Select Input Z/Coupling: 50 Ohm/DC.
  - d Select the Scale field, then enter 40 mV/div.

- e Select the Offset field, then enter 0 V.

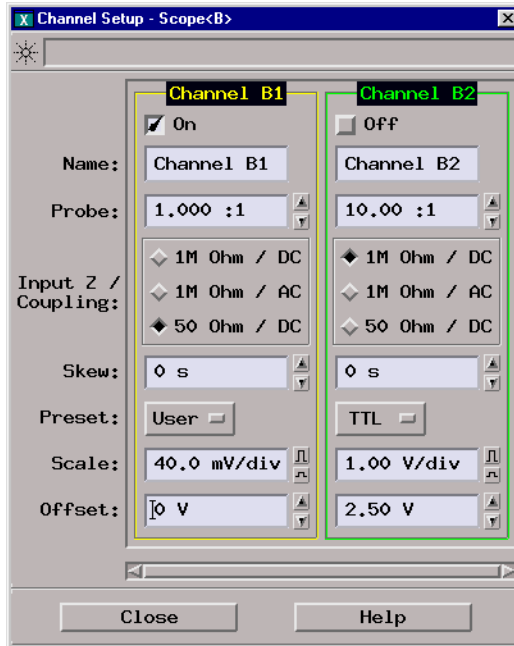


- f Select Close to close the Channel Setup window.
- 3 Set up the Display.
- a In the oscilloscope Setup/Display window, select the Display tab.
- b Select Waveform Mode Average, and set # Avgs: 32.

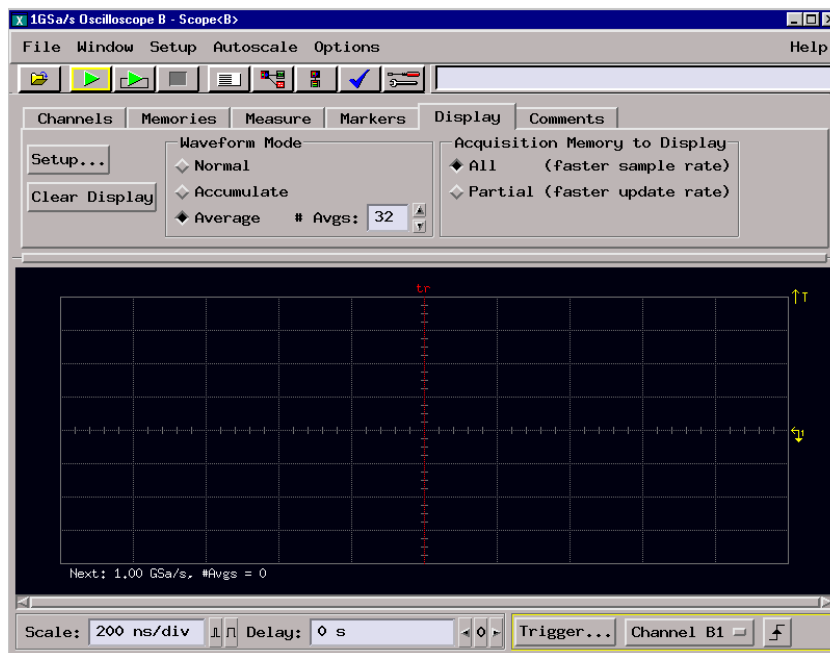

- 4 Set up the Trigger.
- a At the bottom of the display, select Trigger.
- b In the Trigger Setup window, select Mode Edge.
- c Select the Source field, then select Channel 1.

d Select the Level field, then enter 0 V.

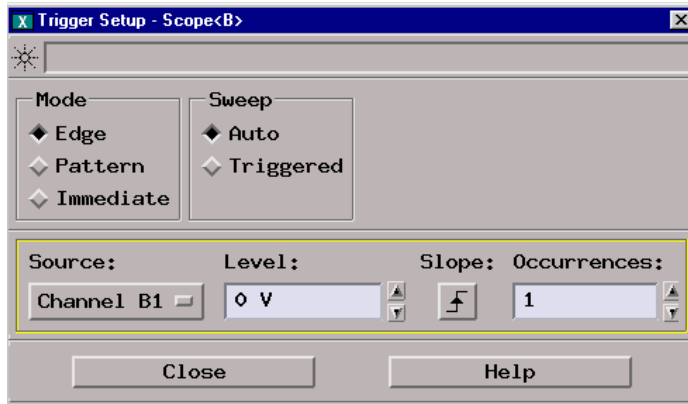


e Select Close to close the Trigger Setup window.

5 Ensure the Markers are turned off.

a In the oscilloscope Setup/Display window, select the Markers tab.

b Under the Markers tab, select Setup. The Markers Setup window opens.

c In the Marker Setup window, ensure all markers are disabled, as shown.

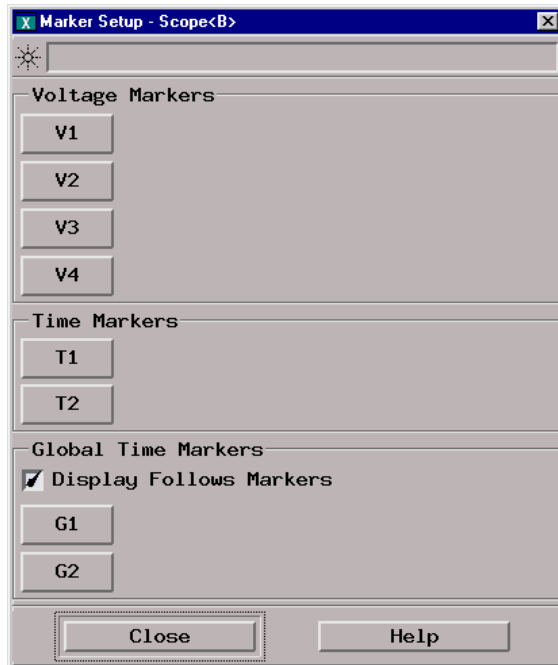


d Select Close to close the Marker Setup window.



---

## Connect the oscilloscope

- 1 Using the N cable, connect the signal generator to the power splitter input. Connect the power sensor to one output of the power splitter.
- 2 Using the N-to-BNC adapter, connect the other power splitter output to the channel 1 input of the oscilloscope.

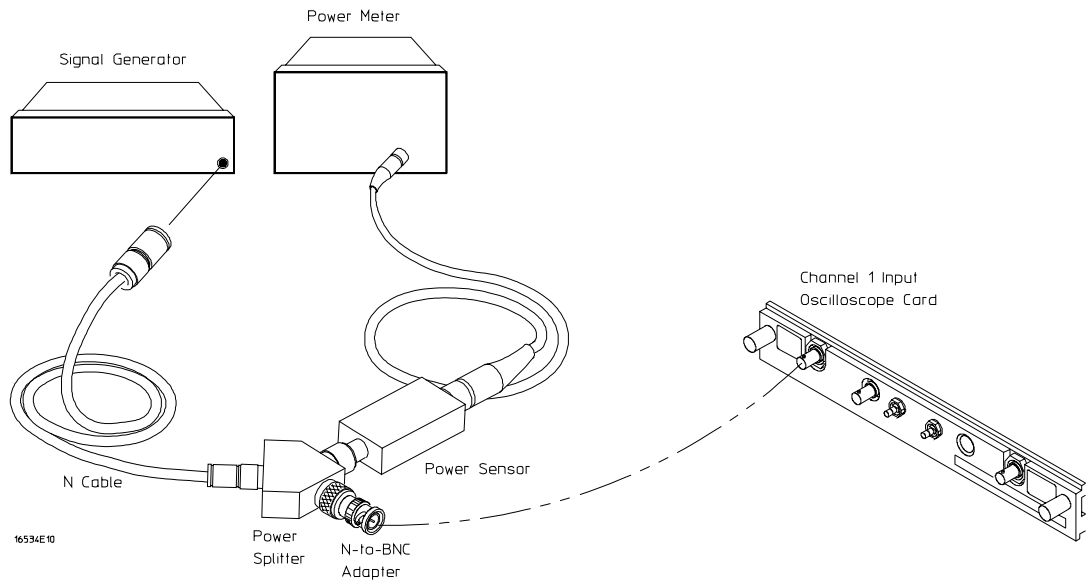

---


## Acquire the data

- 1 Obtain the 1 MHz response.
  - a Set the signal generator for 1 MHz at  $-2.4$  dBm.
  - b Select Run-Repetitive. The signal on the screen should be two cycles at six divisions amplitude. After averaging is complete, select Stop.


Testing Performance  
**To test the bandwidth (16534A only)**

- c In the oscilloscope Setup/Display window, select the Measure tab. Note the voltage reading in the  $V_{p-p}$  field.

$V_1$  MHz = \_\_\_\_\_ mV.

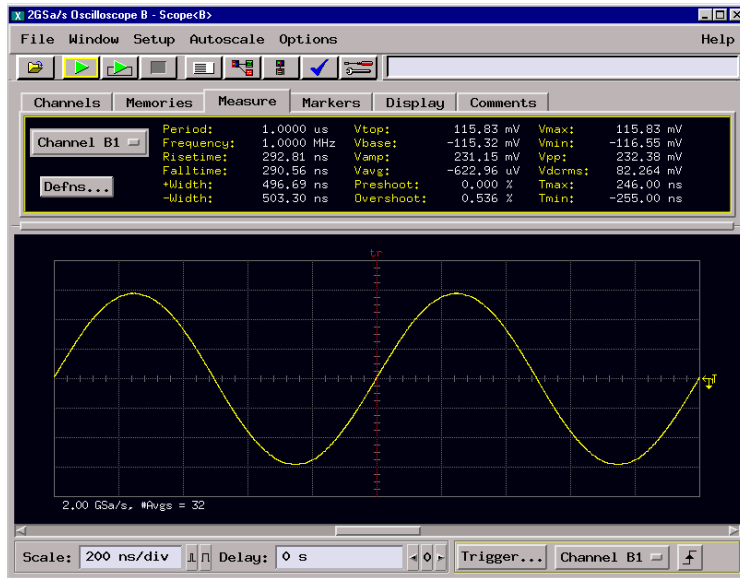

- 2 Set the signal generator for 500 MHz frequency.
  - a Set the power meter Cal Factor % to the 1 MHz value from the calibration chart on the power splitter. Press dB[REF] to set a 0 dB reference.
  - b Change the signal generator frequency to 500 MHz. Set the power meter Cal Factor % to the 500 MHz value from the chart.
  - c Adjust the signal generator amplitude for a power reading as close as possible to 0.0 dB[REL] and note the power reading. Reading = \_\_\_\_\_ dB.
- 3 Obtain the 500 MHz response.
  - a At the bottom of the Setup/Display window, select the Scale field, then enter 1 ns/div.
  - b Select Run-Repetitive. After averaging is complete, select Stop.
  - c Note the voltage reading in the  $V_{p-p}$  field  $V_{500MHz}$  = \_\_\_\_\_ mV.

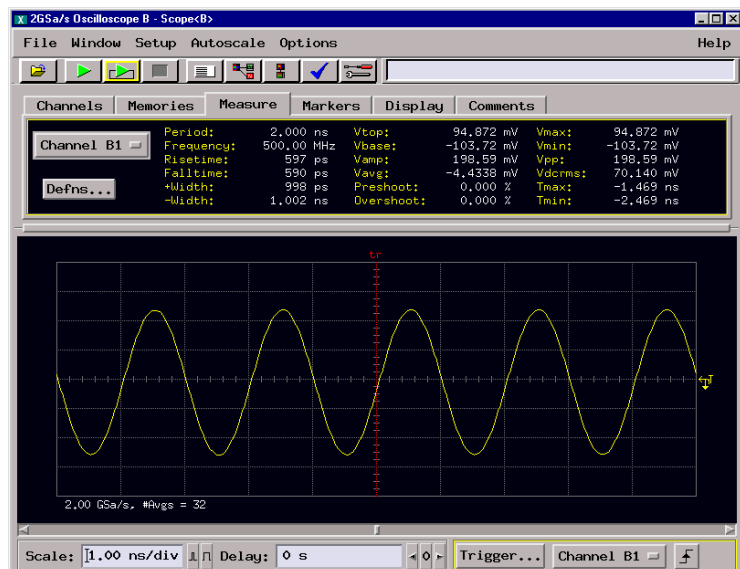

**4** Determine the oscilloscope response.

**a** Calculate the response using the formula:

$$response (dB) = 20 \log_{10} \frac{V_{500MHz}}{V_{1MHz}} = 20 \log_{10} (\text{_____}) = \text{_____} dB$$

**b** Correct the result from step 4a above with any differences in the power meter from step 2c. Observe signs. For example:

Result from step 4a = -1.36 dB

Power meter reading = -0.20 dB[REL]

then true response = (-1.36) - (-0.20) = -1.16dB

$$(\text{_____}) - (\text{_____}) = \text{_____} dB$$

**c** The result from step 4b should be  $\leq -3.0$  dB. Record the result in the performance test record.

**5** Remove the power splitter from the oscilloscope module channel 1 input and connect it to the channel 2 input.

**6** Repeat from "Set up the oscilloscope" for channel 2, replacing channel 1 with channel 2 where applicable.

**See Also**

Failure of the bandwidth test can be caused by a faulty attenuator or main assembly (see chapter 6).

---

## To test the time measurement accuracy

Testing the time measurement accuracy verifies the performance of the following specification:

- **Time Measurement accuracy**

This test uses a precise frequency source to check the accuracy of time measurement functions.

---

### Equipment Required

Equipment	Critical Specifications	Recommended Agilent Model/Part
Signal Generator	200 MHz, timebase accuracy 0.25 ppm	E4400B Option 1E5
Cable	BNC (m)(m) 48-inch	8120-1840
Adapter	Type N (m) to BNC (f)	1250-0780

---


## Set up the equipment

- 1 Turn on the equipment required and the logic analysis system mainframe with the oscilloscope module to be tested. Let them warm up for 30 minutes if you have not already done so.
- 2 Set the signal generator to 181.81818 MHz (5.5 ns period) and approximately 600 mV rms.

---

## Set up the oscilloscope


- 1 Set up the oscilloscope.
  - a In the Logic Analysis System window, select the module icon, then select Setup/Display. The oscilloscope setup/Display window opens.
  - b Select the Channel 2 On field, and the field will toggle to Off.
  - c At the bottom of the Setup/Display window, select the Scale field, then enter 1.00 ns/div.
  - d Select the Delay field, then enter 2.000 ns.

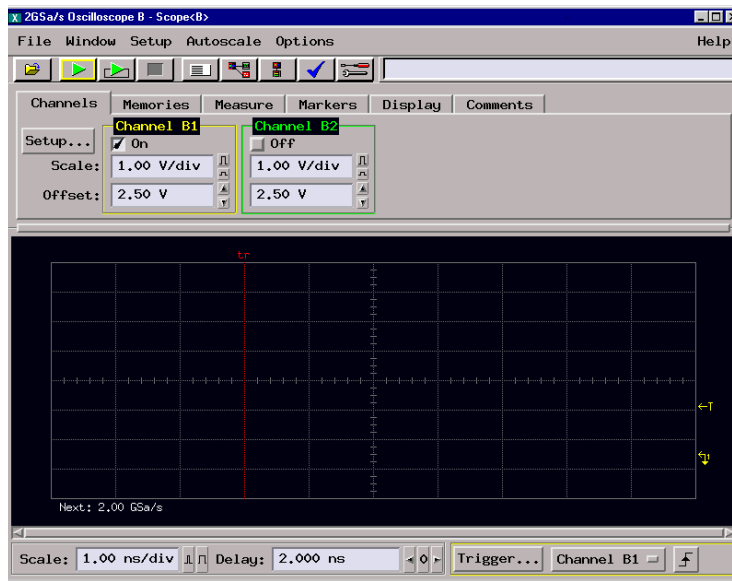

- 2 Set up the Channel.
  - a Under the Channels tab, select Setup. The Channel Setup window opens.
  - b Select the Probe field, then enter 1:1.
  - c Select Input Z/Coupling: 50 Ohm/DC.
  - d Select the Scale field, then enter 200 mV/div.

Testing Performance  
To test the time measurement accuracy


- e Select the Offset field, then enter 0 V.

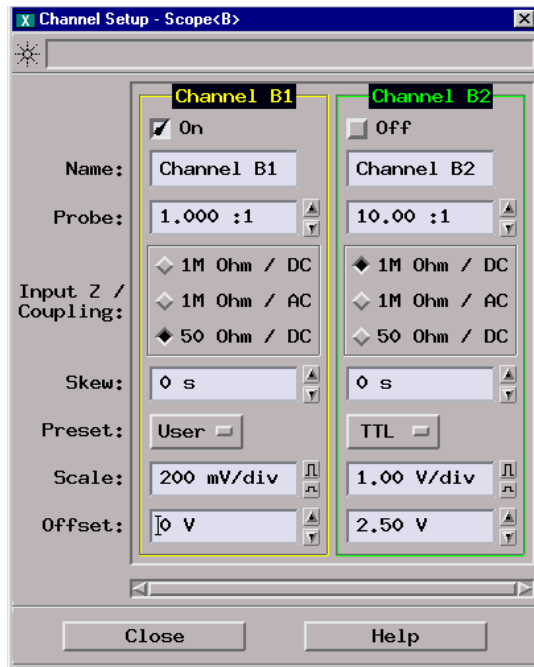

- f Select Close to close the Channel Setup window.

3 Set up the Display.

- a In the oscilloscope Setup/Display window, select the Display tab.

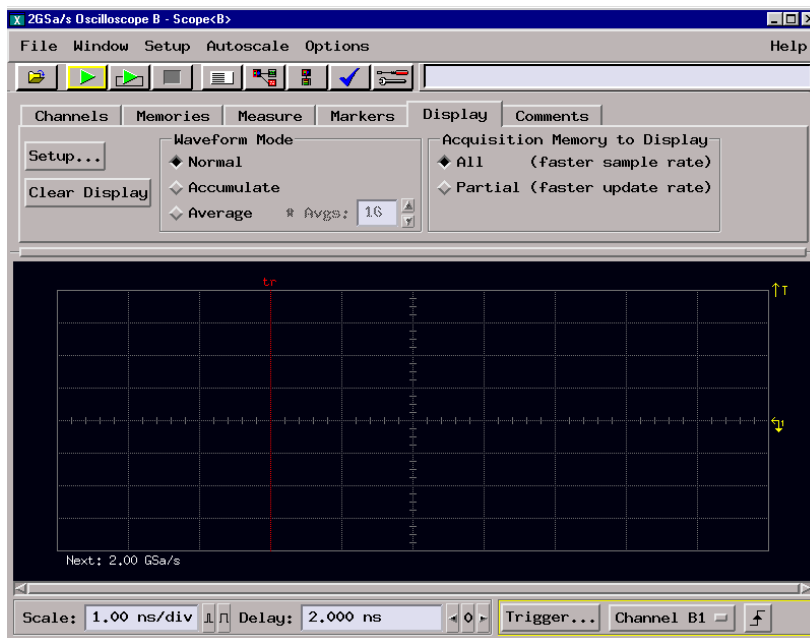


- b Select Waveform Mode Normal.

4 Set up the Trigger.


- a At the bottom of the display, select Trigger.
- b In the Trigger Setup window, select Mode Edge.

- c Select the Source field, then select Channel 1.
- d Select the Level field, then enter 0 V.

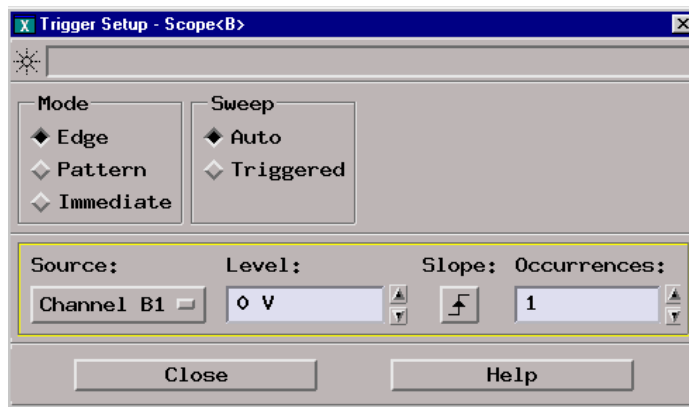

- e Select Close to close the Trigger Setup window.
- 5 Set up the Markers.
- a In the oscilloscope Setup/Display window, select the Markers tab.
  - b Under the Markers tab, select Setup. The Markers Setup window opens.
  - c In the Markers Setup window, select T1, then select Automatic. T1-Automatic will be enabled.
  - d In the Marker Setup window, select Define Automatic Marker. Set the T1 Automatic Marker parameters according to the following table:

Source	Channel 1
Type	%
Level	50%
Slope	Positive
Edge#	1

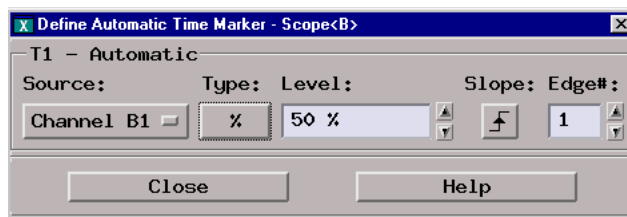

- e Select Close to close the Define Automatic Marker window for T1.
- f In the Marker Setup window, select T2, then select Automatic. T2-Automatic will be enabled.

Testing Performance  
**To test the time measurement accuracy**

**g** In the Marker Setup window, select Define Automatic Marker. Set the T2 Automatic Marker parameters according to the following table:

Source	Channel 1
Type	%
Level	50%
Slope	Positive
Edge#	2




- h** Select Close to close the Define Automatic Marker window for T2.
- i** Select Close to close the Marker Setup window.

---

## Connect the oscilloscope


Using the N-to-BNC adapter and the BNC cable, connect the signal generator output to the channel 1 input of the oscilloscope.

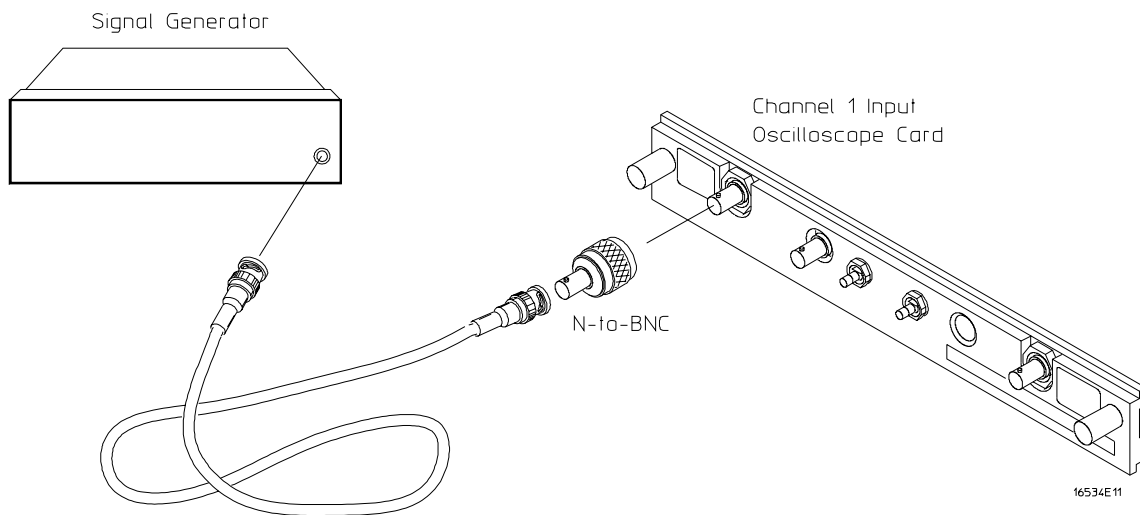



## Acquire the data


- 1 Determine short time period accuracy.
  - a Select Run-Repetitive. If the waveform is clipping, reduce the signal generator output voltage level until the waveform no longer clips. After approximately two minutes, touch Stop.
  - b Under the Markers tab, check to see that the Mean T2 - T1 field is approximately 5.500 ns. Check that both the Min T2 - T1 and the Max T2 - T1 are within 100 ps of the Mean T2 - T1. Record the results in the performance test record.

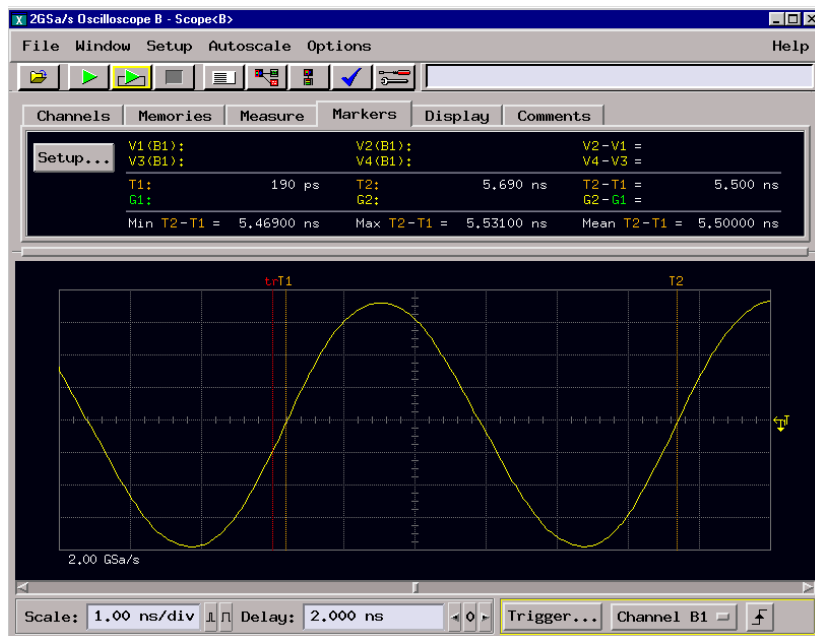


- 2 Determine the longer time period accuracy.
  - a Select Stop to halt the acquisition.
  - b Under the Markers tab, select Setup.

Testing Performance  
To test the time measurement accuracy

- c Select T1-Auto, then select Automatic to turn off Automatic T1 measurements.

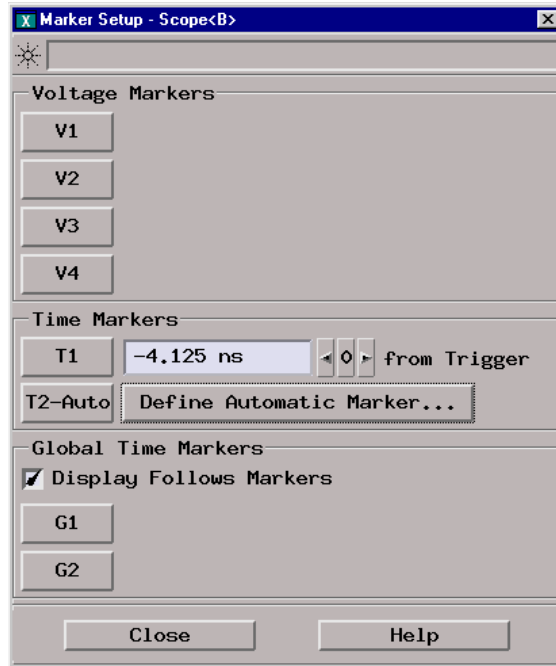


- d Select Define Automatic Marker for T2. At the Define Automatic Marker window, select Edge# 1.

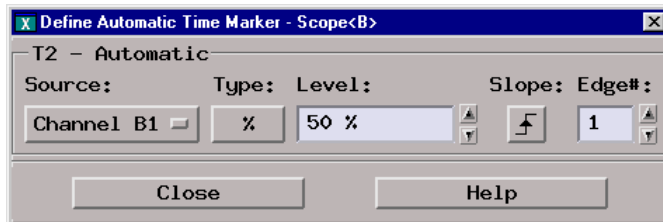

- e Select Close to close the Define Automatic Marker window for T2.

f In the oscilloscope Setup/Display window, select the Delay field, then enter 687.500 ns.

Ensure a rising edge appears at the left of the display, and the T2 - T1 time is approximately 687.5 ns.

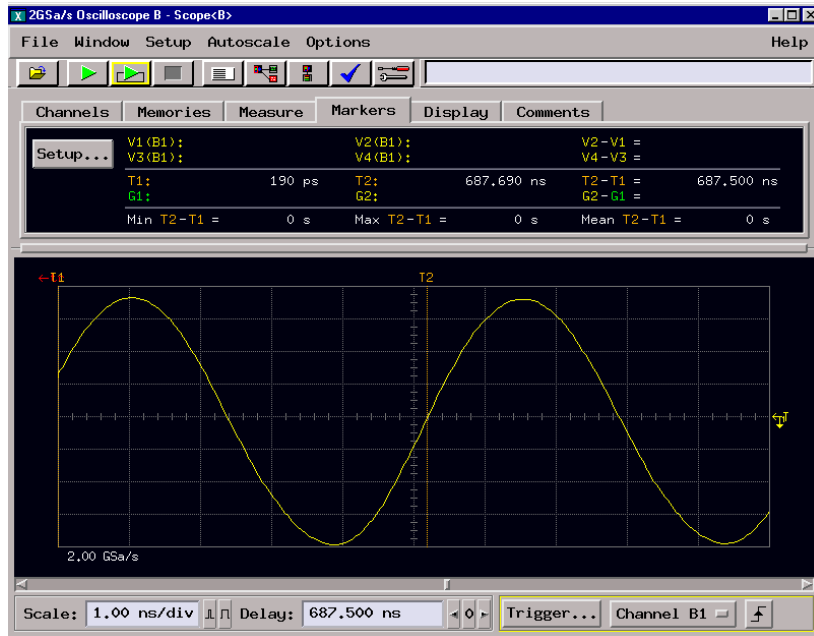

g Record the T2 - T1 time in the Performance Test Record.

---

## To test the trigger sensitivity (16533A only)

Testing the trigger sensitivity verifies the performance of the following specifications:

- DC to 50 MHz: 0.063 x full scale (0.5 division)
- 50 to 250 MHz: 0.125 x full scale (1.0 division)

---

### Equipment Required

---

Equipment	Critical Specifications	Recommended Agilent Model/Part
Signal Generator	50 and 225 MHz, 30 - 80 mV RMS output	E4400B Option 1E5
Cable	BNC 48-inch	8120-1840
Adapter	Type N (m) to BNC (f)	1250-0780

---


### Set up the equipment

Turn on the equipment required and the logic analysis system mainframe with the oscilloscope module to be tested. Let them warm up for 30 minutes if you have not already done so.

---

## Set up the oscilloscope


- 1 Set up the oscilloscope.
  - a In the Logic Analysis System window, select the module icon, then select Setup/Display. the oscilloscope setup/Display window opens.
  - b Select the Channel 2 On field, and the field will toggle to Off.
  - c At the bottom of the Setup/Display window, select the Scale field, then enter 2.00 ns/div.

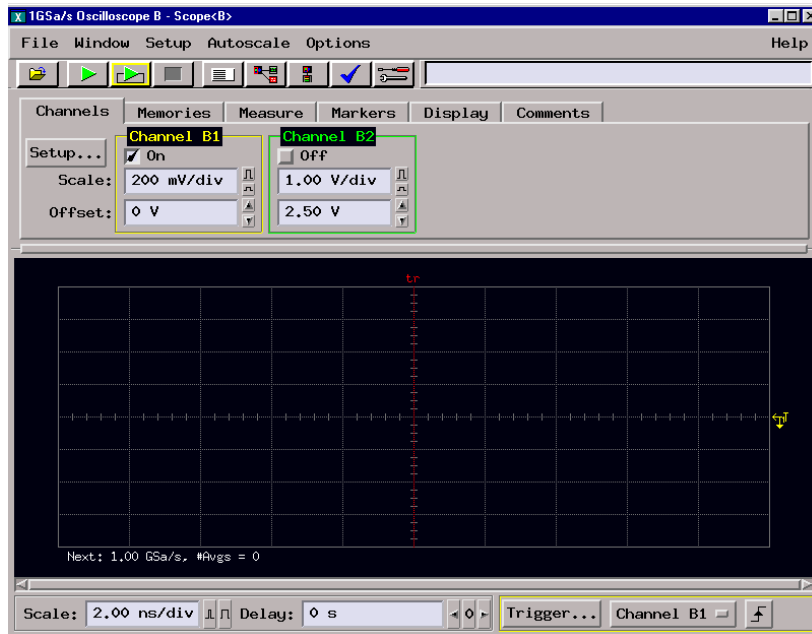

- 2 Set up the Channel.
  - a Under the Channels tab, select Setup. The Channel Setup window opens.
  - b Select the Probe field, then enter 1.000:1.
  - c Select Input Z/Coupling: 50 Ohm/DC.
  - d Select the Scale field, then enter 200 mV/div.

Testing Performance  
To test the trigger sensitivity (16533A only)

e Select the Offset field, then enter 0 V.

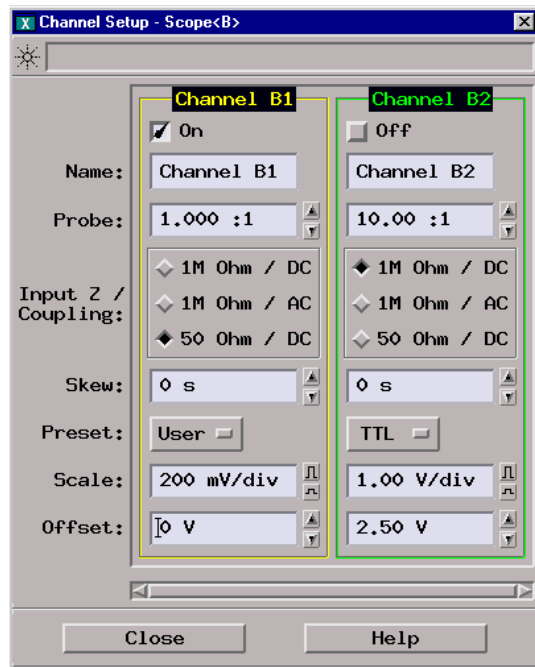


f Select Close to close the Channel Setup window.

3 Set up the Display.

a In the oscilloscope Setup/Display window, select the Display tab.

b Select Waveform mode Average, and set # Avgs: 16.

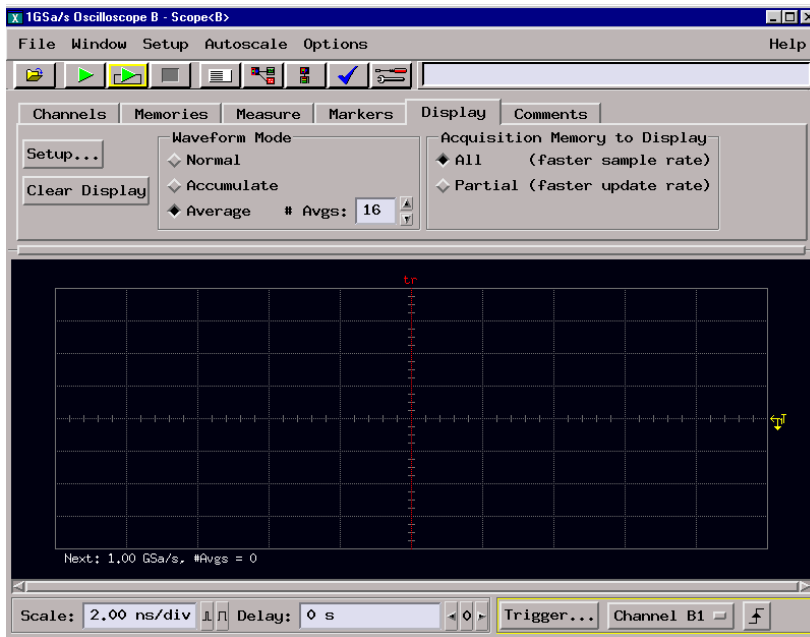


4 Set up the Trigger.


a At the bottom of the display, select Trigger.

b In the Trigger Setup window, select Mode Edge.

- c Select Sweep Triggered.
- d Select the Source field, then select Channel 1.
- e Select the Level field, then enter 0 V.

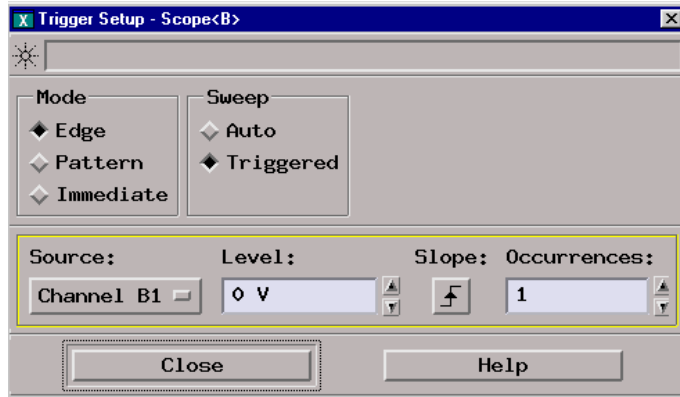

- f Select Close to close the Trigger Setup window.
- 5 Ensure the Markers are turned off.
- a In the oscilloscope Setup/Display window, select the Markers tab.
  - b Under the Markers tab, select Setup. The Markers Setup window opens.
  - c In the Marker Setup window, ensure all markers are disabled, as shown.

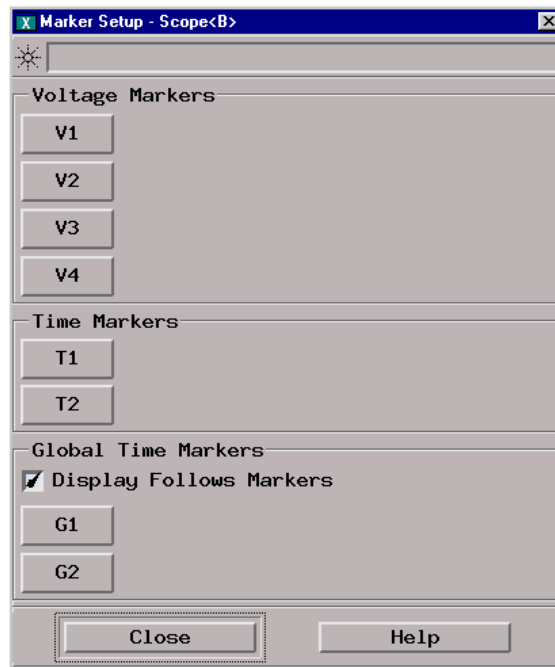


- d Select Close to close the Marker Setup window.

---

## Connect the oscilloscope

Using the N-to-BNC adapter and the BNC cable, connect the signal generator output to the channel 1 input of the oscilloscope.

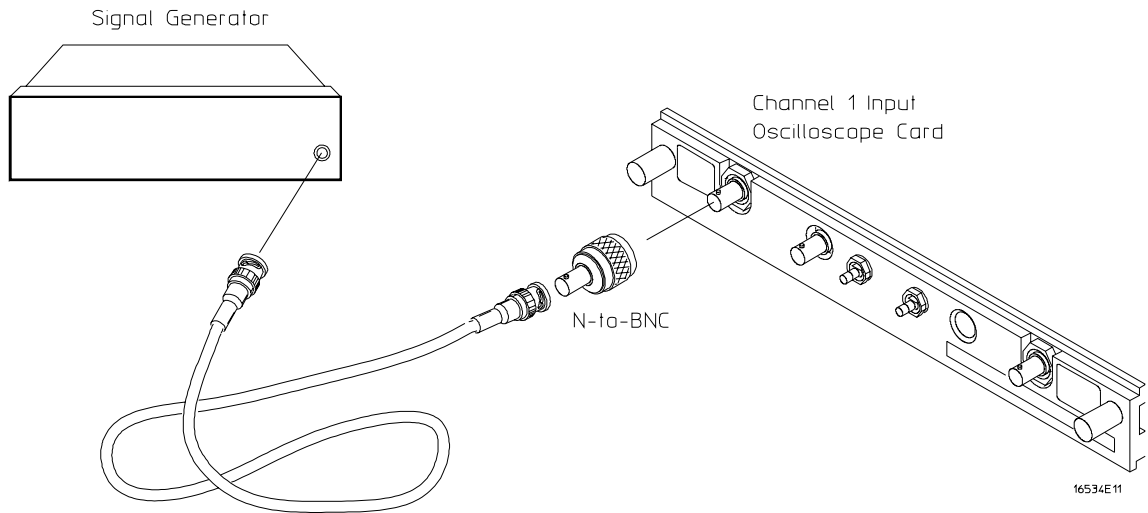

---

## Acquire the data

- 1 Test the upper bandwidth trigger sensitivity.
  - a Set the signal generator to provide a 225 MHz signal with 70 mV rms amplitude.
  - b Select Run-Repetitive. In the oscilloscope Setup/Display window, select the Measure tab Adjust the signal generator amplitude until the Vp-p field displays 200 mV (maximum).

---

**Note** If the Waiting for Trigger message appears, change the Trigger level. To change the Trigger level, position the mouse cursor over the Trigger level markers (←T) Then click and drag the Trigger level marker up and down until the oscilloscope triggers.

---



- c If the oscilloscope triggers, record a pass in the performance test record. Select Stop to halt the acquisition.



- 2 Test the lower bandwidth trigger sensitivity.
- In the oscilloscope Setup/Display window, select the Scale field and enter 20 ns/div.
  - Set the signal generator to provide a 50 MHz signal. Set the signal generator's amplitude to one-half the current setting (from upper bandwidth trigger sensitivity).
  - Select Run-Repetitive. Adjust the signal generator amplitude until the Vp-p field displays 100 mV (maximum).

**Note**

If the Waiting for Trigger message appears, change the Trigger level. To change the Trigger level, position the mouse cursor over the Trigger level markers (←T) Then click and drag the Trigger level marker up and down until the oscilloscope triggers.

Testing Performance  
To test the trigger sensitivity (16533A only)

d If the oscilloscope triggers, record a pass in the performance test record.



- e Select Stop to halt the acquisition.
- 3 Remove the signal generator output from channel 1 and connect the BNC cable to channel 2. Repeat from "Set up the oscilloscope" for channel 2, replacing channel 1 with channel 2 where appropriate.

---

## To test the trigger sensitivity (16534A only)

Testing the trigger sensitivity verifies the performance of the following specifications:

- DC to 50 MHz: 0.063 x full scale (0.5 division)
- 50 to 500 MHz: 0.125 x full scale (1.0 division)

---

### Equipment Required

---

Equipment	Critical Specifications	Recommended Agilent Model/Part
Signal Generator	50 and 450 MHz, 30 - 80 mV RMS output	E4400B Option 1E5
Cable	BNC 48-inch	8120-1840
Adapter	Type N (m) to BNC (f)	1250-0780


---

### Set up the equipment

Turn on the equipment required and the logic analysis system mainframe with the oscilloscope module to be tested. Let them warm up for 30 minutes if you have not already done so.


## Set up the oscilloscope

- 1 Set up the oscilloscope.
  - a In the Logic Analysis System window, select the module icon, then select Setup/Display. The oscilloscope Setup/Display window opens.
  - b Select the Channel 2 On field, and the field will toggle to Off.
  - c At the bottom of the Setup/Display window, select the Scale field, then enter 2.00 ns/div.

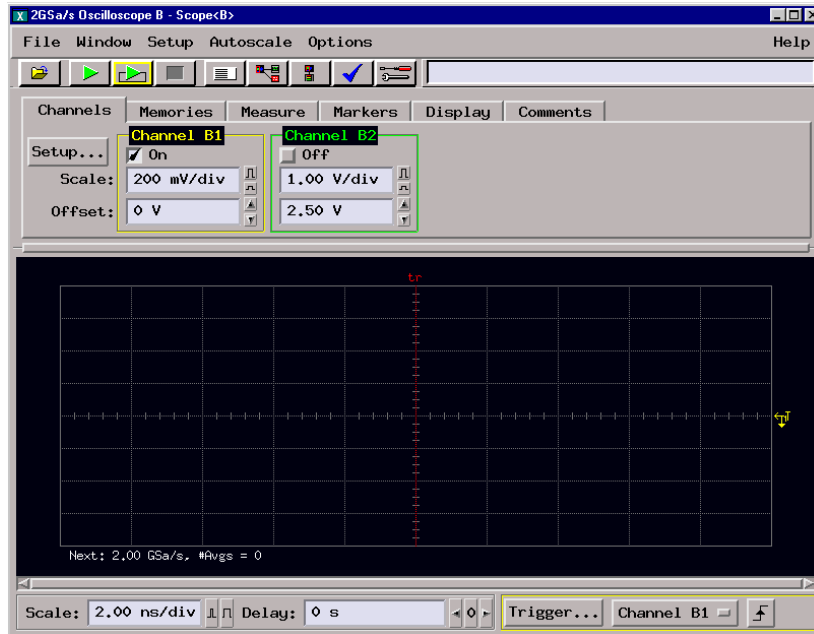

- 2 Set up the Channel.
  - a Under the Channels tab, select Setup. The Channel Setup window opens.
  - b Select the Probe field, then enter 1.000:1.
  - c Select Input Z/Coupling: 50 Ohm/DC.
  - d Select the Scale field, then enter 200 mV/div.

e Select the Offset field, then enter 0 V.

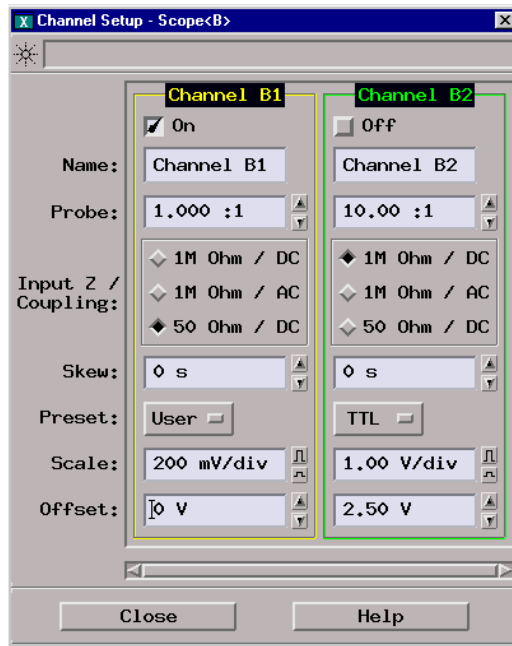


f Select Close to close the Channel Setup window.

3 Set up the Display.

a In the oscilloscope Setup/Display window, select the Display tab.

b Select Waveform Mode Average, and set # Avgs: 16.

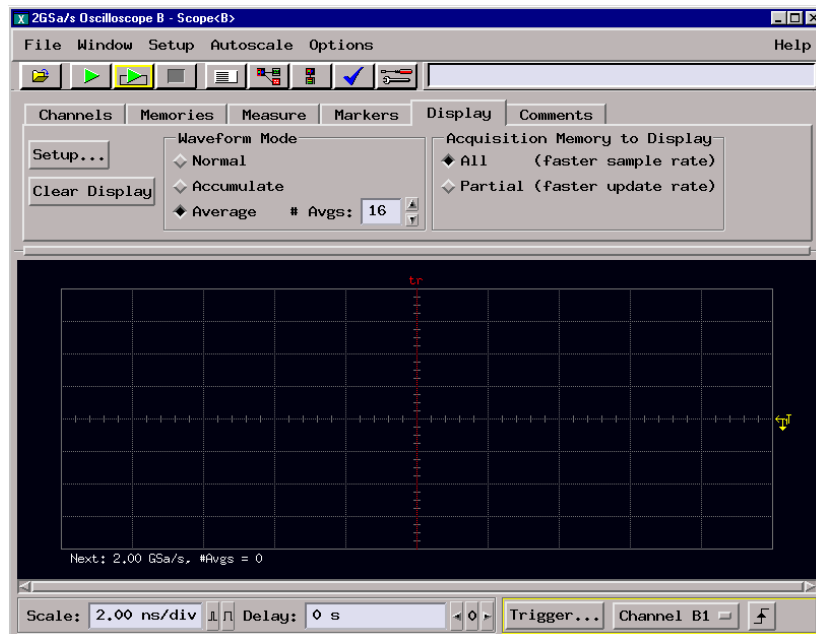

4 Set up the Trigger.


a At the bottom of the display, select Trigger.

b In the Trigger Setup window, select Mode Edge.


c Select Sweep Triggered.

Testing Performance  
To test the trigger sensitivity (16534A only)

- d Select the Source field, then select Channel 1.
- e Select the Level field, then enter 0 V.

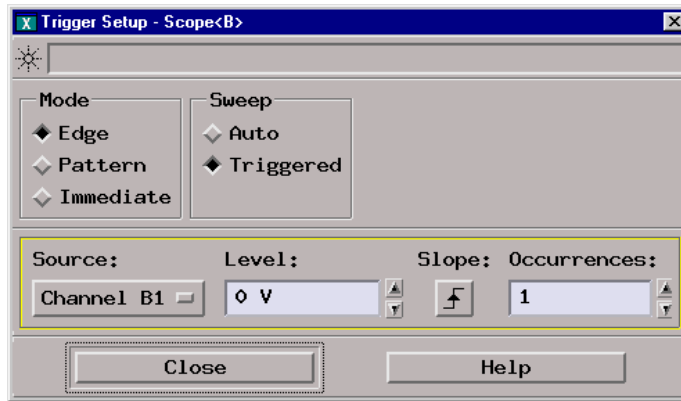

- f Select Close to close the Trigger Setup window.
- 5 Ensure the Markers are turned off.
- a In the oscilloscope Setup/Display window, select the Markers tab.
  - b Under the Markers tab, select Setup. The Markers Setup window opens.
  - c In the Marker Setup window, ensure all markers are disabled, as shown.

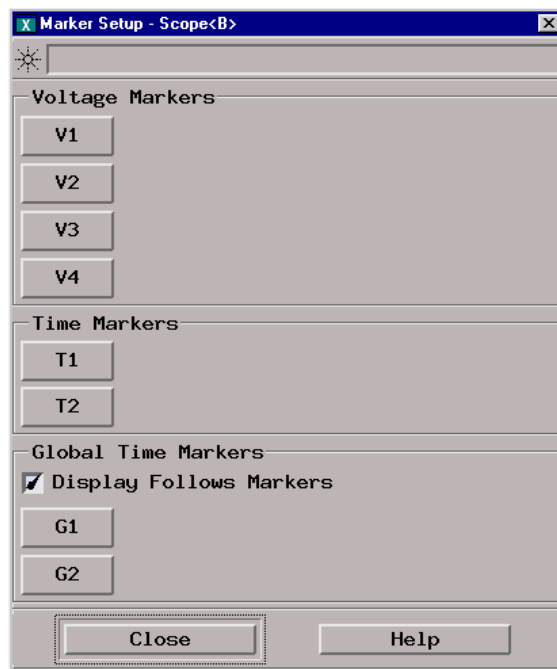


- d Select Close to close the Marker Setup window.

---

## Connect the oscilloscope

Using the N-to-BNC adapter and the BNC cable, connect the signal generator output to the channel 1 input of the oscilloscope.

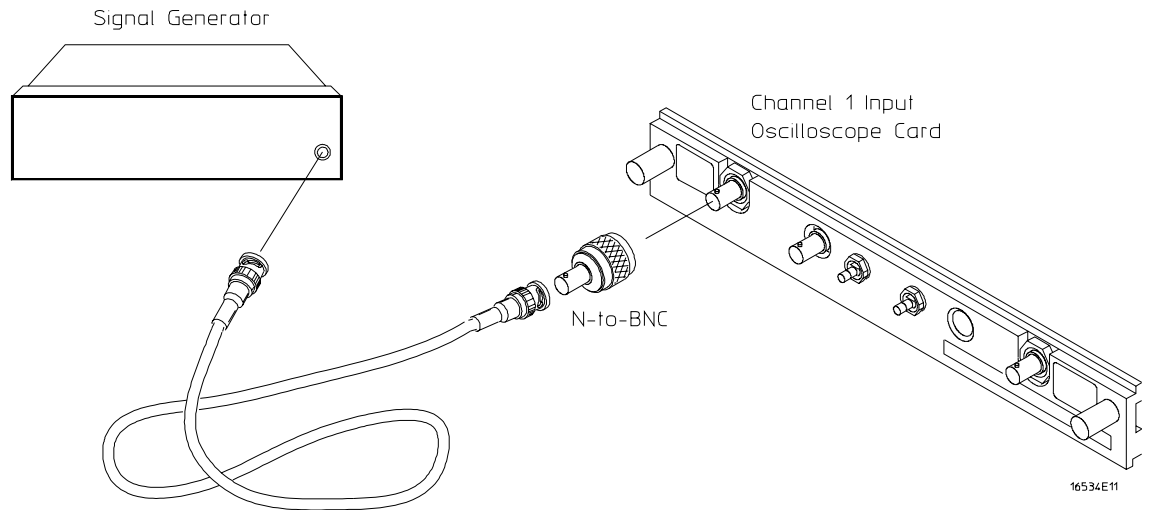

---

## Acquire the data

- 1 Test the upper bandwidth trigger sensitivity.
  - a Set the signal generator to provide a 450 MHz signal with 70 mV rms amplitude.
  - b Select Run-Repetitive. In the oscilloscope Setup/Display window, select the Measure tab. Adjust the signal generator amplitude until the Vp-p field displays 200 mV (maximum).


---

### Note

If the Waiting for Trigger message appears, change the Trigger level. To change the Trigger level, position the mouse cursor over the Trigger level makers (←T) Then click and drag the Trigger level marker up and down until the oscilloscope triggers.

Testing Performance  
To test the trigger sensitivity (16534A only)

- c If the oscilloscope triggers, record a pass in the performance test record. Touch Stop to halt the acquisition.

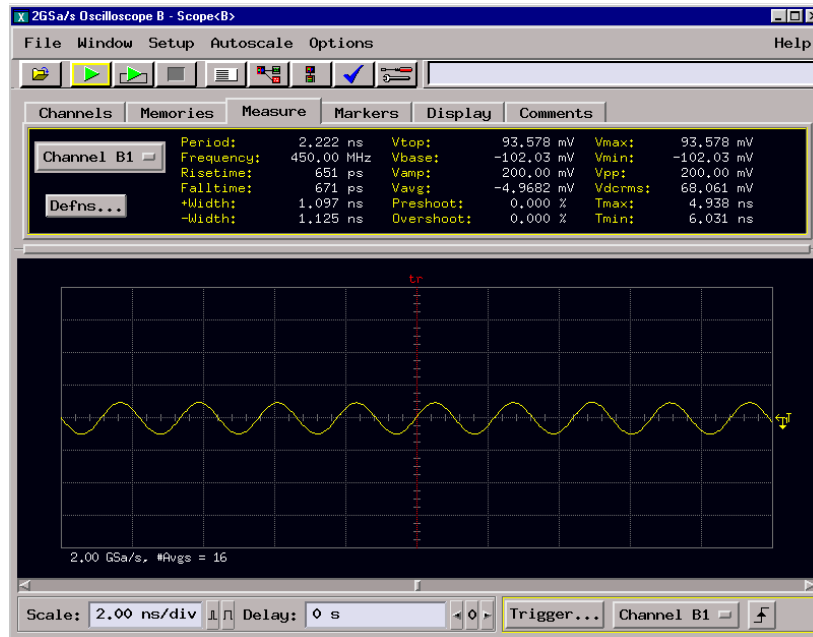

- 2 Test the lower bandwidth trigger sensitivity.
- a In the oscilloscope Setup/Display window, select the Scale field and enter 20 ns/div.
  - b Set the signal generator to provide a 50 MHz signal. Set the signal generator's amplitude to one-half the current setting (from upper bandwidth trigger sensitivity).
  - c Select Run-Repetitive. Adjust the signal generator amplitude until the Vp-p field displays 100 mV (maximum).

**Note** If the Waiting for Trigger message appears, change the Trigger level. To change the Trigger level, position the mouse cursor over the Trigger level markers (←T) Then click and drag the Trigger level marker up and down until the oscilloscope triggers.



d If the oscilloscope triggers, record a pass in the performance test record.



e Select Stop to halt the acquisition.

- 3 Remove the signal generator output from channel 1 and connect the BNC cable to channel 2. Repeat from "Set up the oscilloscope" for channel 2, replacing channel 1 with channel 2 where appropriate.

---

## Performance Test Record

Serial No. _____ Recommended Test Interval - 2 Year/4000 hours Recommended next testing _____	<b>16533A/34A Oscilloscope</b> _____ Work Order No. _____ Date _____ Temperature _____
---	---

Test	Settings	Results
<b>Self-Tests</b>		Pass/Fail _____
<b>Input Resistance</b>	50 Ω ± 0.5 Ω (49.5 to 50.5 Ω) 1 MΩ ± 10 KΩ (0.990 to 1.010 MΩ)	
<b>Channel 1</b>		50 Ω @ 20 mV/Div _____ 1 MΩ @ 20 mV/Div _____ 50 Ω @ 200 mV/Div _____ 1 MΩ @ 200 mV/Div _____ 50 Ω @ 1 V/Div _____ 1 MΩ @ 1 V/Div _____ 50 Ω @ 5 V/Div _____ 1 MΩ @ 5 V/Div _____
<b>Channel 2</b>		50 Ω @ 20 mV/Div _____ 1 MΩ @ 20 mV/Div _____ 50 Ω @ 200 mV/Div _____ 1 MΩ @ 200 mV/Div _____ 50 Ω @ 1 V/Div _____ 1 MΩ @ 1 V/Div _____ 50 Ω @ 5 V/Div _____ 1 MΩ @ 5 V/Div _____
<b>Operational Accuracy Calibration</b>		Pass/Fail _____

Test	Settings	Results					
<b>Voltage Measurement Accuracy</b>		Limits	Measured				
		<b>Channel 1</b>	<b>Scale</b>	<b>Offset</b>			
			5 V/div	-17.5 V	-34.340 V to -35.660 V	_____	
			1 V/div	-3.5 V	-6.868 V to -7.132 V	_____	
			200 mV/div	-700.0 mV	-1.374 V to -1.426 V	_____	
			40 mV/div	-140 mV	-274.8 mV to -285.2 mV	_____	
			40 mV/div	140 mV	285.2 mV to 274.8 mV	_____	
			200 mV/div	700.0 mV	1.426 V to 1.374 V	_____	
			1 V/div	3.5 V	7.132 V to 6.868 V	_____	
			5 V/div	17.5 V	35.660 V to 34.340 V	_____	
		<b>Channel 2</b>	<b>Scale</b>	<b>Offset</b>			
			5 V/div	-17.5 V	-34.340 V to -35.660 V	_____	
			1 V/div	-3.5 V	-6.868 V to -7.132 V	_____	
			200 mV/div	-700.0 mV	-1.374 V to -1.426 V	_____	
			40 mV/div	-140 mV	-274.8 mV to -285.2 mV	_____	
			40 mV/div	140 mV	285.2 mV to 274.8 mV	_____	
			200 mV/div	700.0 mV	1.426 V to 1.374 V	_____	
			1 V/div	3.5 V	7.132 V to 6.868 V	_____	
			5 V/div	17.5 V	35.660 V to 34.340 V	_____	
		<b>Offset Accuracy</b>	<b>Zero-input offset</b>				
				<b>Channel 1</b>	5 V/div	0.00 V±800.0 mV	_____
					1 V/div	0.00 V±160.0 mV	_____
					200 mV/div	0.00 V±32.0 mV	_____
	40 mV/div			0.00 V±6.4 mV	_____		
<b>Channel 2</b>	5 V/div			0.00 V±800.0 mV	_____		
	1 V/div			0.00 V±160.0 mV	_____		
	200 mV/div			0.00 V±32.0 mV	_____		
	40 mV/div			0.00 V±6.4 mV	_____		
	<b>Scale</b>			<b>Offset</b>			
<b>Channel 1</b>	1 V/div			-35.00 V	-34.490 V to -35.510 V	_____	
	200 mV/div			-10.00 V	-9.868 V to -10.132 V	_____	
	40 mV/div			-2.00 V	-1.9736 V to -2.0264 V	_____	
	40 mV/div			+2.00 V	2.0264 V to 1.9736 V	_____	
	200 mV/div			+10.00 V	10.132 V to 9.868 V	_____	
	1 V/div			+35.00 V	35.510 V to 34.490 V	_____	
<b>Channel 2</b>	1 V/div			-35.00 V	-34.490 V to -35.510 V	_____	
	200 mV/div			-10.00 V	-9.868 V to -10.132 V	_____	
	40 mV/div			-2.00 V	-1.9736 V to -2.0264 V	_____	
	40 mV/div			+2.00 V	2.0264 V to 1.9736 V	_____	
	200 mV/div			+10.00 V	10.132 V to 9.868 V	_____	
	1 V/div			+35.00 V	35.510 V to 34.490 V	_____	

Testing Performance  
Performance Test Record

Test	Settings	Results	
<b>Bandwidth</b>		Limit	Measured
<b>Channel 1</b>		≤-3.0dB	_____
<b>Channel 2</b>		≤-3.0dB	_____
<b>Time Measurement Accuracy</b>	5.500ns ± 100ps	Min T2 - T1	_____
		Max T2 - T1	_____
		Mean T2 - T1	_____
	687.500ns ± 135ps	T2 - T1	_____
<b>16533A Trigger Sensitivity</b>			
<b>Channel 1</b>	Trigger Stable @ 225 MHz (200mVp_p max) Trigger Stable @ 50 MHz (100mVp_p max)	Pass/Fail	_____
<b>Channel 2</b>	Trigger Stable @225 5 MHz (200mVp_p max) Trigger Stable @ 50 MHz (100mVp_p max)	Pass/Fail	_____
<b>16534A Trigger Sensitivity</b>			
<b>Channel 1</b>	Trigger Stable @ 450 MHz (200mVp_p max) Trigger Stable @ 50 MHz (100mVp_p max)	Pass/Fail	_____
<b>Channel 2</b>	Trigger Stable @450 5 MHz (200mVp_p max) Trigger Stable @ 50 MHz (100mVp_p max)	Pass/Fail	_____

Calibrating and Adjusting

Oscilloscope calibration 4-2

Multicard oscilloscope Calibration 4-2

To calibrate the oscilloscope 4-3

Self Cal calibrations 4-4

Protect the operational accuracy calibration factors 4-8

Load the default calibration factors 4-8

To Deskew the Channel-to-Channel Variations 4-9

---

# Calibrating and Adjusting

This chapter gives you instructions for calibrating and adjusting the oscilloscope. The calibration and adjustment procedures in this chapter are for both the Agilent Technologies 16533A and 16534A.

To periodically verify the performance of the analyzer against specifications, refer to "Testing Performance" in chapter 3.

---

## Oscilloscope calibration

The oscilloscope circuitry in the 16533A/34A oscilloscope requires an operational accuracy calibration by the user or service department under any of the following conditions:

- at six months intervals or every 1,000 hours
- if the ambient temperature changes more than 10° C from the temperature at full calibration
- to optimize measurement accuracy

To test the oscilloscope circuitry against specifications (full calibration), refer to chapter 3, Testing Performance.

---

## Multicard oscilloscope calibration

A complete operational accuracy calibration on an 16533A/34A multicard module requires the module to first be separated into single card modules. The operational accuracy calibrations on the acquisition subsystem are done on the single card modules. After reconfiguring the 16533A/34A module into a multicard module, the channel skew calibration is done.

# To calibrate the oscilloscope

## Equipment Required

Equipment	Critical Specification	Recommended Agilent Model/Part	Qty
Cable (2)	BNC, 9-inch (equal length)	8120-1838	2
Adapter	BNC (m)(m)	1250-1236	1
Adapter	BNC tee (m)(f)(f)	1250-0781	1
Adapter	BNC (f)/SMB (m)	1250-1236	1

## Set up the equipment


### CAUTION

The effects of ELECTROSTATIC DISCHARGE can damage components. Use grounded wrist straps and mats when you are performing any kind of service on this module.

The 16533A/34A oscilloscope module contains a calibration PROTECT/UNPROTECT switch. This switch must be set to UNPROTECT before new calibration values from the operational accuracy calibration can be stored to nonvolatile RAM.

16533A/34A multicard modules must be separated into single card modules before performing the operational accuracy calibration on the acquisition circuitry.

- 1 Remove power from the instrument. If a multicard module is being calibrated, Disconnect all Master/Expander Trigger Cables from the ECL EXT TRIG IN and OUT connectors on the rear panel of each 16533A/34A card.
- 2 Pull out halfway all cards and filler panels located above the oscilloscope, then remove the filler panels and cards located above the oscilloscope.
- 3 Remove the 16533A/34A module and set the PROTECT/UNPROTECT switch to the UNPROTECT position. On a multicard module, the PROTECT/UNPROTECT switch on all cards must be set to UNPROTECT.

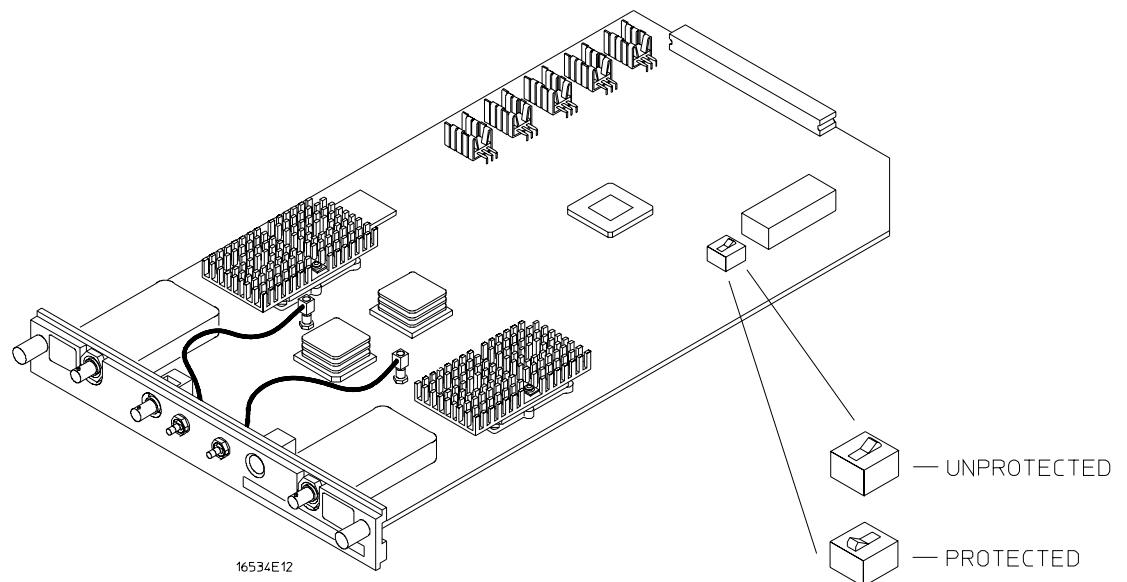

- 4 Reinstall the modules and filler panels.
- 5 Apply power to the Agilent Technologies 16700-series logic analysis system. Allow the 16533A/34A module to warm up approximately 30 minutes before doing the following steps.

---

## Self Cal calibrations

- 1 Begin the operational accuracy calibration.


Note that once the default calibration factors are loaded, all calibrations must be done. The calibration must be performed in the exact sequence listed below.

---

### NOTE

The calibration PROTECT/UNPROTECT switch on the 16533A/34A oscilloscope module must be set to UNPROTECT.


- a In the Logic Analysis System window, select the module icon for the 16533A/34A to be calibrated, then select Calibration. The oscilloscope Calibration window opens.
- b In the Calibration window, select Default Factors. At the confirmation, select Yes to load the default calibration factors.

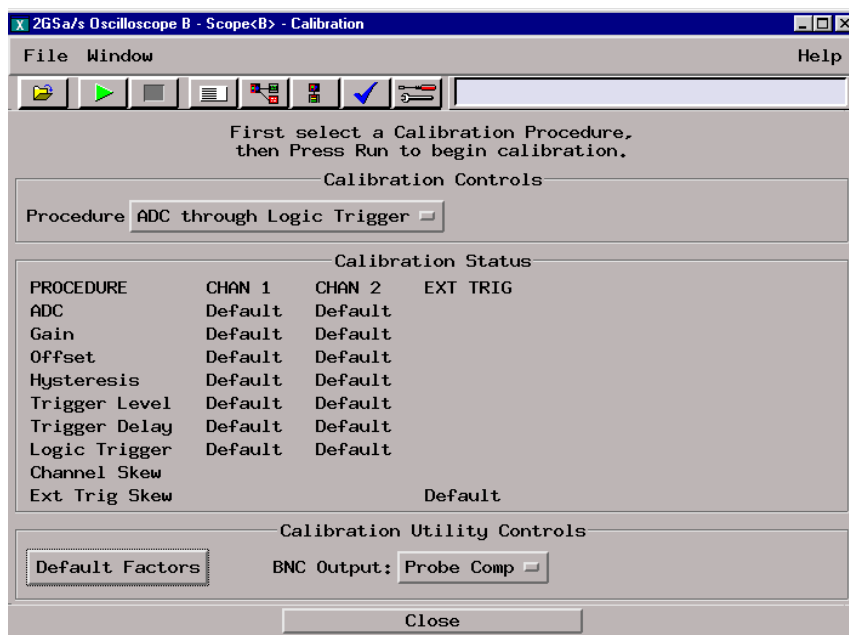

- c Connect two BNC 50-ohm, 9-inch cables to the BNC tee adapter. Once you select Run, the instrument will prompt you to connect the cables to the appropriate locations on the rear panel of the module.
- d Select the Run icon, then follow the instructions in the display.



Messages will be displayed as each operational accuracy calibration routine is completed to indicate calibration has passed or failed. The resulting calibration factors are automatically stored to nonvolatile RAM at the conclusion of each calibration routine.

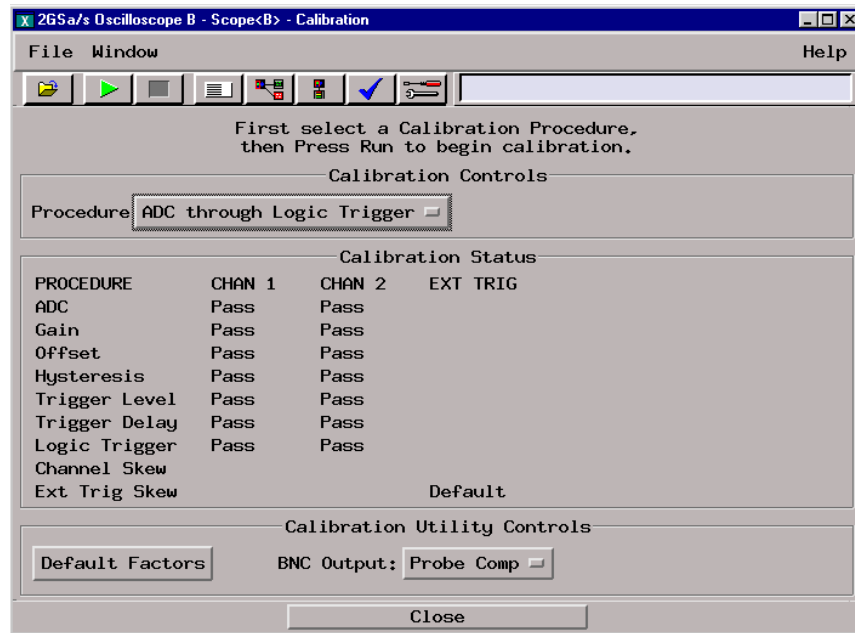

**2 Do the External Trigger Skew operational accuracy calibration.**

- a Select the Procedure field, then at the pop-up select Ext Trig Skew.
- b Connect BNC 50-ohm, 9-inch cables to one side of the BNC tee adapter. Connect the BNC 50-ohm(f)/SMB(m) adapter to the other side of the BNC tee adapter using a BNC(m) (m) adapter. Once you select Run, the instrument will prompt you to connect the cables to the appropriate locations on the rear panel of the module.




Calibrating and Adjusting  
To calibrate the oscilloscope

- c Select the Run icon, then follow the instructions on the display. When the Ext Trig Skew calibration is complete, the resulting calibration factors are stored in non-volatile RAM.



- d After completion of the External Trigger Skew calibration, remove the cables from the instrument.
- 3 If a multcard 16533A/34A module is being calibrated, repeat steps 1 and 2 for the next 16533A/34A card until all cards have been completed.
- 4 If a multcard 16533A/34A module is being calibrated, perform the following steps to reconfigure the multcard module before proceeding to step 5.
- a Select Close to close the Calibration window.
  - b In the Logic Analysis System window, select File, then select Exit to close the logic analyzer session.
  - c In the Session Manager, select Shutdown. In the window, select Powerdown.
  - d When the "OK to powerdown" message appears, turn off the power switch.

- e Install the Master/Expander Trigger Cables in the ECL EXT TRIG IN and OUT connectors on the rear panel of each 16533/34a card. Starting with the top-most 16533/34A card, connect the ECL EXT TRIG OUT to the ECL TRIG IN of the card immediately below. Repeat for all cards in the module.

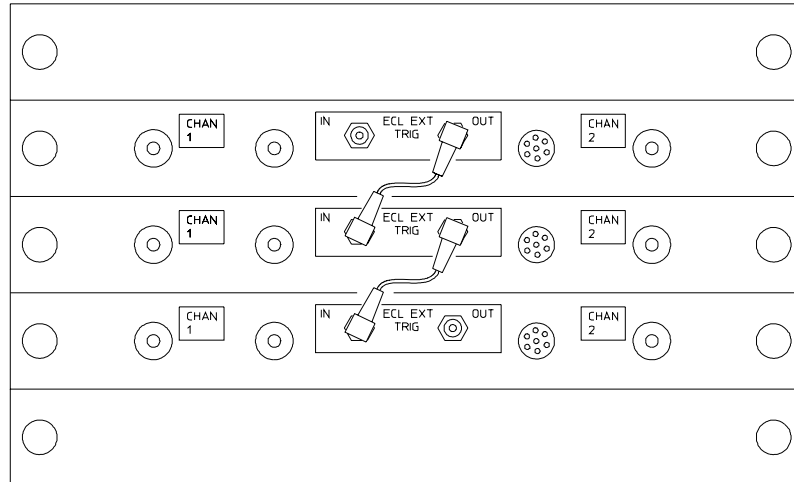

16534E04

- f Reapply power to the 16700-series mainframe.
  - g After powerup is complete, select the icon of the master 16533A/34A card of the multicard module. Select Calibration. The oscilloscope Calibration window opens.
- 5 Do the channel skew calibration on the multicard module.
- a Connect two BNC 50-ohm, 9-inch cables to the BNC tee adapter. Once you select Run, the instrument will prompt you to connect the cables to the channels selected in the Calibration window.
  - b In the Calibration window, select the Channels field. Select two channels to deskew.



- c Select the Run icon, then follow the instructions on the display.
- d Repeat steps b and c until all channel combinations have been deskewed.

---

## Protect the operational accuracy calibration factors

- 1 Remove power from the instrument. Pull out halfway all cards and filler panels located above the oscilloscope.
- 2 Remove the 16533A/34A module and set the PROTECT/UNPROTECT switch to the PROTECT position. On a multicard module, the PROTECT/UNPROTECT switch on all cards must be set to PROTECT.
- 3 Reinstall the modules and filler panels.

---

## Load the default calibration factors

If data displayed by the 16533A/34A oscilloscope module appears to be incorrect and the calibration factors stored by the operational accuracy calibration factors is suspect, the default calibration factors can be loaded. Loading the default calibration factors can be used in this way to verify the 16533A/34A oscilloscope module hardware is operating properly and that an operational accuracy calibration should be performed.


Note that once the default calibration factors are loaded, all calibrations must be done. In a multicard 16533A/34A, the cards must be separated into single card modules to do the operational accuracy calibrations on the acquisition circuitry.

---

### NOTE

The calibration PROTECT/UNPROTECT switch on the 16533A/34A oscilloscope module must be set to UNPROTECT.

- 1 In the Logic Analysis System window, select the module icon for the 16533A/34A to be calibrated, then select Calibration. The oscilloscope Calibration window opens.
- 2 In the Calibration window, select Default Factors. At the confirmation, select Yes to load the default calibration factors.

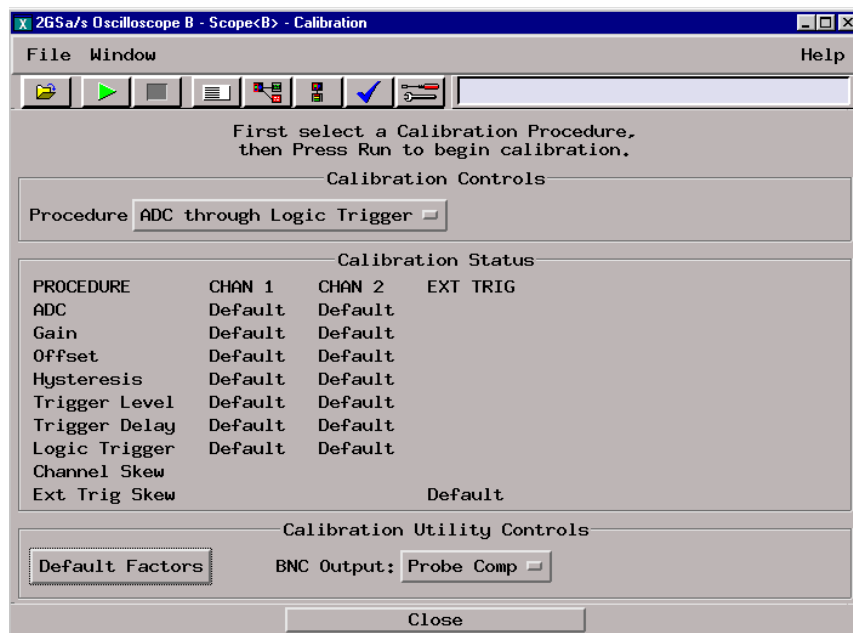


## To deskew the channel-to-channel variations

Deskewing the channel-to-channel variations sets the timing of all channels to correspond to channel 1 at the probe tip. This eliminates time discrepancies between channels caused by variations in cable lengths. Also, you can use deskew to manually adjust for any differences in cable length by horizontally overlaying displayed waveforms that are time-skewed. The oscilloscope module channels are deskewed in 1 ps increments up to the maximum value of +/- 100 ns.

This procedure uses the probe compensation signal from the rear panel calibration port as a signal source for channel-to-channel deskewing. However, any signal source can be used for this procedure.

### 1 Set up the oscilloscope.

- a In the Logic Analysis System window, select the module icon for the 16533A/34A to be deskewed, then select Setup/Display. The oscilloscope Setup/Display window opens.

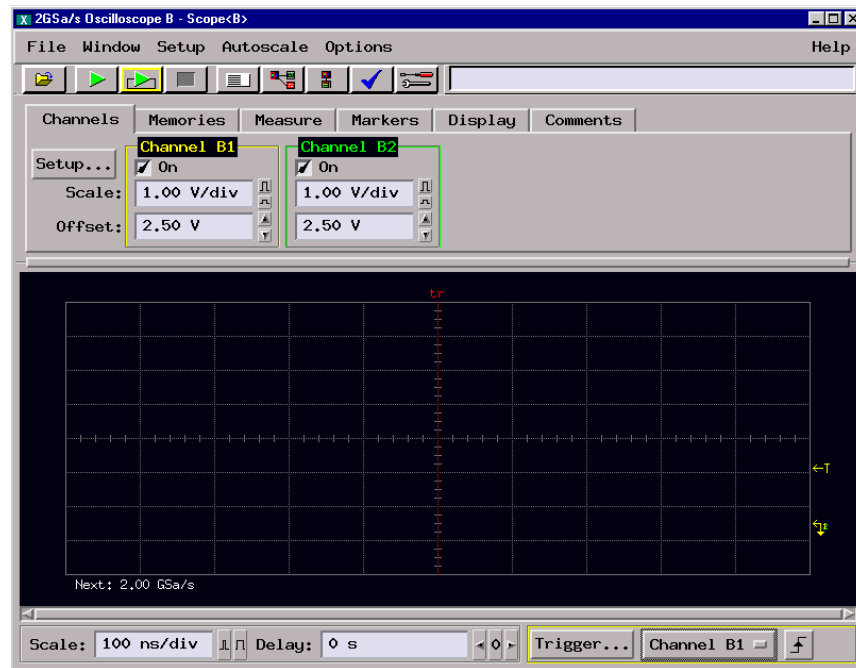

- b Connect the male end of a BNC "Tee" adapter to the calibration signal port on the rear panel of the oscilloscope module.
- c Connect Channel 1 of the oscilloscope module to one side of the BNC "Tee" adapter. Use any other adapters necessary to provide a good connection to the BNC "Tee."
- d Connect Channel 2 of the oscilloscope module to to one side of the BNC "Tee" adapter. Use any other adapters necessary to provide a good connection to the BNC "Tee."

Note that the oscilloscope probes can be used in place of the BNC cables. Connect the probes to the BNC "Tee" adapter using BNC to probe adapter.


### 2 Deskew the Channel

- a In the oscilloscope Setup/Display window under the Channels tab, select Setup. The Channel Setup window opens.

## Calibrating and Adjusting To calibrate the oscilloscope

Note that if oscilloscope probes are being used, ensure the Probe and Coupling fields in the oscilloscope Channel Setup window are properly set to match the oscilloscope probes being used.

- b** Select the Channel 1 Probe field, then enter 1.000:1.
- c** Select the Channel 2 Input Z/Coupling field, then select 50 Ohm/DC.
- d** Repeat steps b and c for Channel 2.
- e** In the oscilloscope Setup/Display window, select Autoscale. In the popup menu, select Continue.

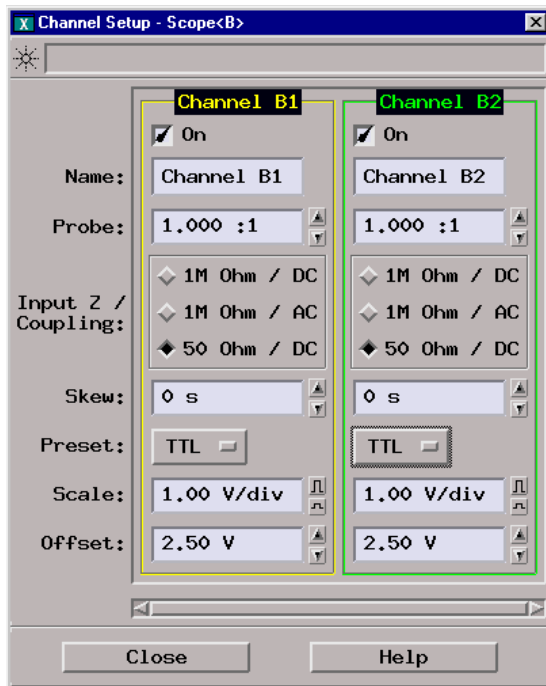


After Autoscale is complete, ensure the Scale and Offset values are the same for Channel 1 and Channel 2 in the Channel Setup menu.

- f In the oscilloscope Setup/Display window, decrease the Scale V/div setting until the channel is measurable.




- g In the oscilloscope Channel Setup window, select the Skew field for either Channel 1 or Channel 2. Change the value until both edges are aligned on the display.

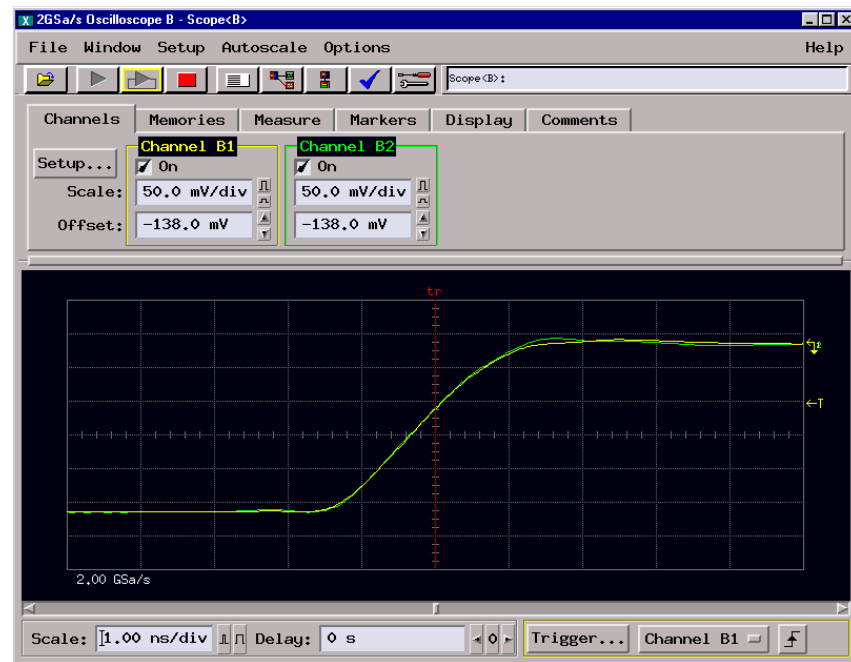

## Calibrating and Adjusting To calibrate the oscilloscope

For this example, Channel 2 Skew was increased to a value of 400 ps.

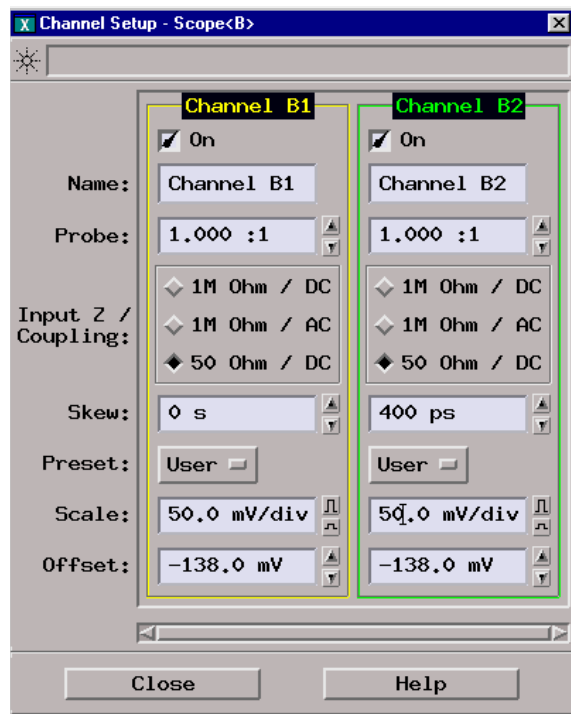

- 3 Select Stop to halt the acquisition.
- 4 If a multcard module is being deskewed, repeat the above procedures for any other channels that you desire to deskew.



Troubleshooting

To use the flowcharts 5-2

To run the self-tests 5-5

To verify the CAL OUTPUT port 5-6

Set up the equipment 5-6

Set up the oscilloscope 5-7

Verify the cal DC output voltages 5-8

Set up the oscilloscope 5-9

Verify the AC CAL OUTPUT 5-10

---

# Troubleshooting

This chapter helps you troubleshoot the oscilloscope to find defective assemblies. The troubleshooting consists of flowcharts, self-test instructions, and tests. This information is not intended for component-level repair.

If you suspect a problem, start at the top of the first flowchart. During the troubleshooting instructions, the flowcharts will direct you to perform other tests.

The service strategy for this instrument is the replacement of defective assemblies. This instrument can be returned to Agilent Technologies for all service work, including troubleshooting. Contact your nearest Agilent Technologies Sales Office for more details.

---

**CAUTION**


---

Electrostatic discharge can damage electronic components. Use grounded wriststraps and mats when you perform any service to this instrument or to the cards in it.

---


## To use the flowcharts

Flowcharts are the primary tool used to isolate defective assemblies. The flowcharts refer to other tests to help isolate the trouble. The circled letters on the charts indicate connections with the other flowcharts. Start your troubleshooting at the top of the first flowchart.

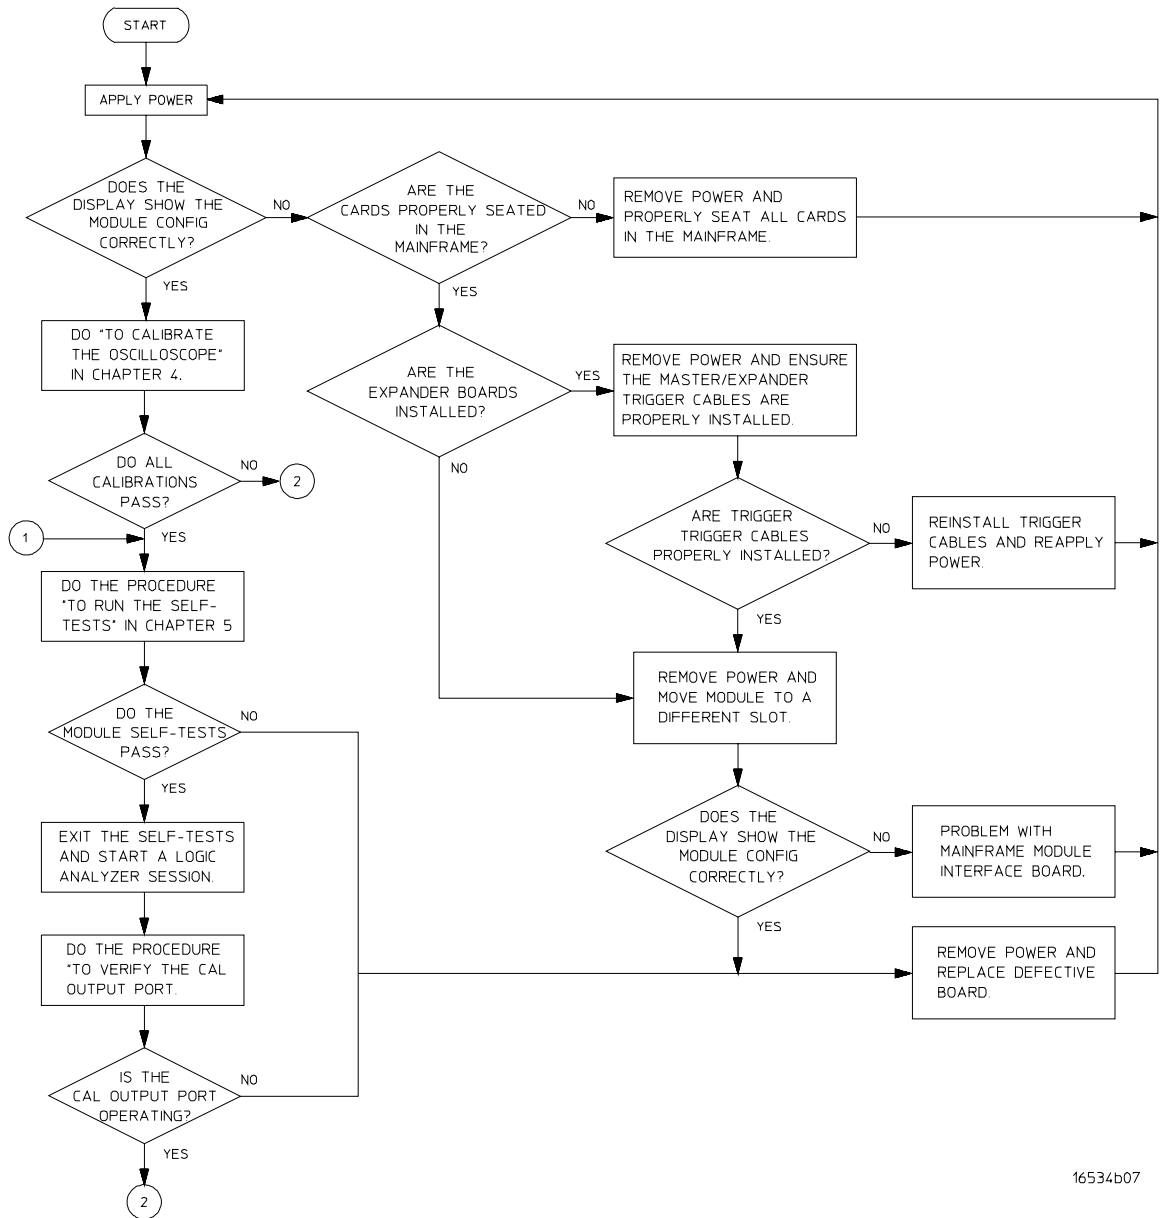

16534b07

**Troubleshooting Flowchart 1**

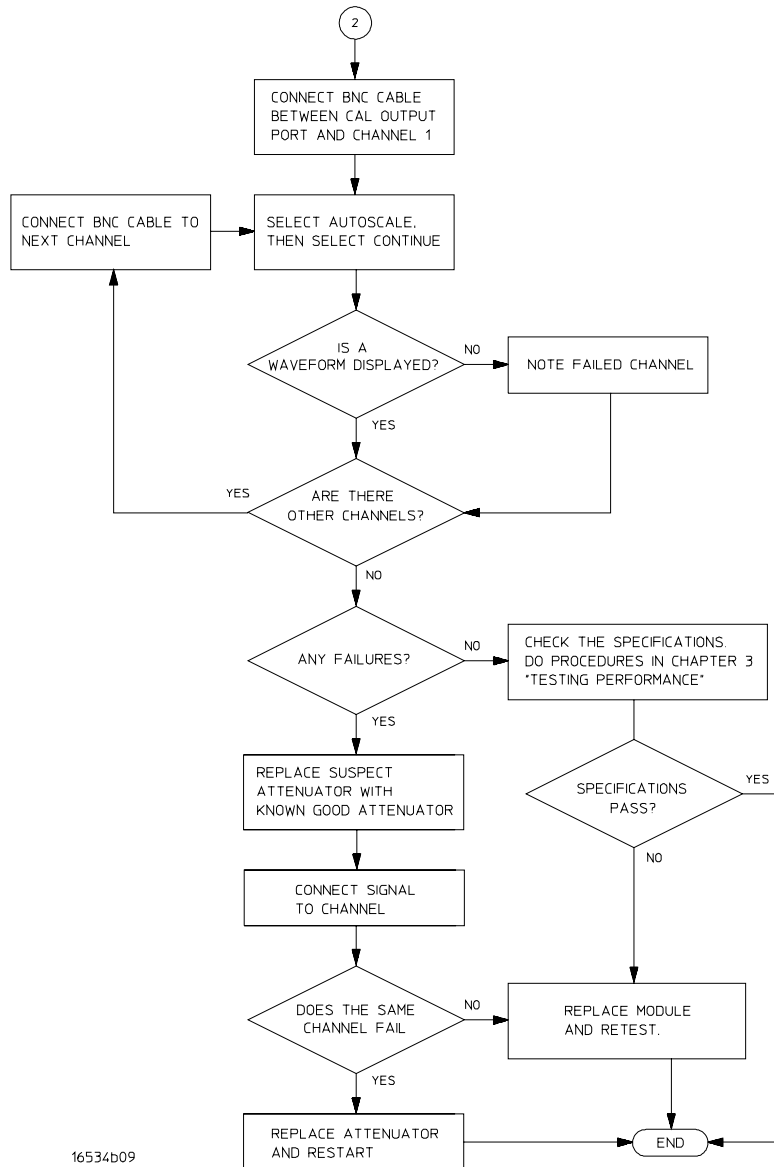

16534b09

**Troubleshooting Flowchart 2**

## To run the self-tests

Self-tests identify the correct operation of major, functional subsystems of the module. You can run all self-tests without accessing the module. If a self-test fails, the troubleshooting flowcharts instruct you to change a part of the module.

To run self-tests:


- 1 In the System window, select System Admin.
- 2 In the System Administration window, select the Admin tab, then select Self Test. At the Test Query window, select Yes.

The tests can be run individually, or all the tests can be run by selecting Test All at the bottom of the Self Test window. Note that if Test All is selected, system tests requiring user action will not be run. For more information, refer to Chapter 8 in the mainframe service manual.

- 3 In the Self Test window under the System tab, select System CPU Board.
- 4 Run the floppy drive test.
  - a In the Self Test window under the System tab, select System CPU Board.
  - b Insert a DOS-formatted disk with 300KB of available space in the mainframe floppy drive.
  - c In the Test Query window, select OK.

The Test Query window instructs you to insert the disk into the disk drive. The other System CPU Board tests require similar user action to successfully run the test.

- 5 In the Self Test: System CPU Board window, select Close to close the window.
- 6 In the Self Test window, select PCI Board. Select Test All to run all PCI board tests.
- 7 In the Self Test window, select the Master Frame tab. Select the 16533A/34A module to be tested, then select Test All to run all the module tests.

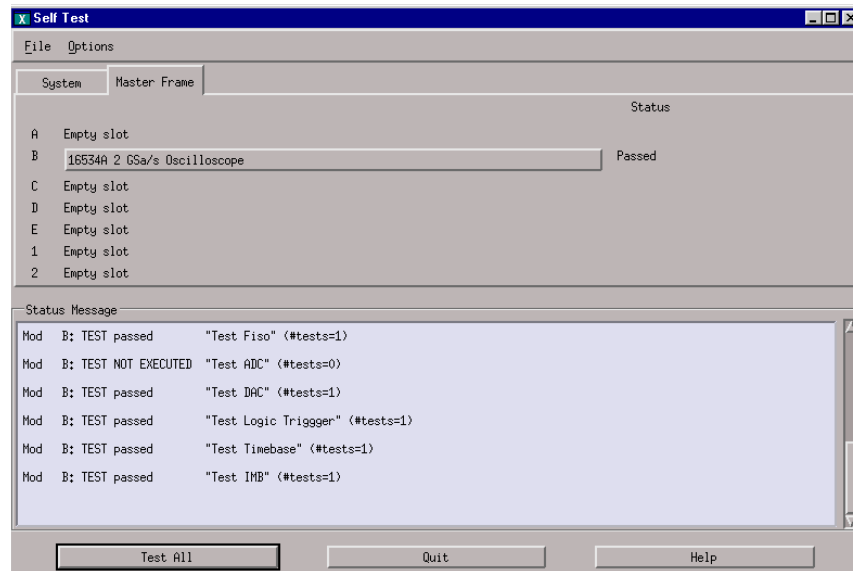

Refer to Chapter 8 in the mainframe service guide for more information on system tests that not executed.

## To verify the CAL OUPUT port

Testing the cal ouput post checks the following:

- dc cal output voltage
- ac cal output voltage

This test verifies that the calibration output voltages are operating, so that they can provide good signal source for the instrument operational accuracy calibration and probe calibration.

---

### Equipment Required

Equipment	Critical Specifications	Recommended Agilent Mode/Part
Digital Multimeter	0.1 mV resolution, better than 0.005% accuracy	3458A
Cable	BNC (m)(m) 48-inch	8120-1840
Adapter	BNC (f) to Dual Banana Plug	1251-2277


---

## Set up the equipment

Turn on the equipment required and the logic analysis system mainframe with the oscilloscope module to be tested. Let them warm up for 30 minutes if you have not already done so.

## Set up the oscilloscope

- 1 Set up the Calibration menu.
  - a In the Logic Analysis System window, select the module icon, then select Calibration. The Calibration window opens.

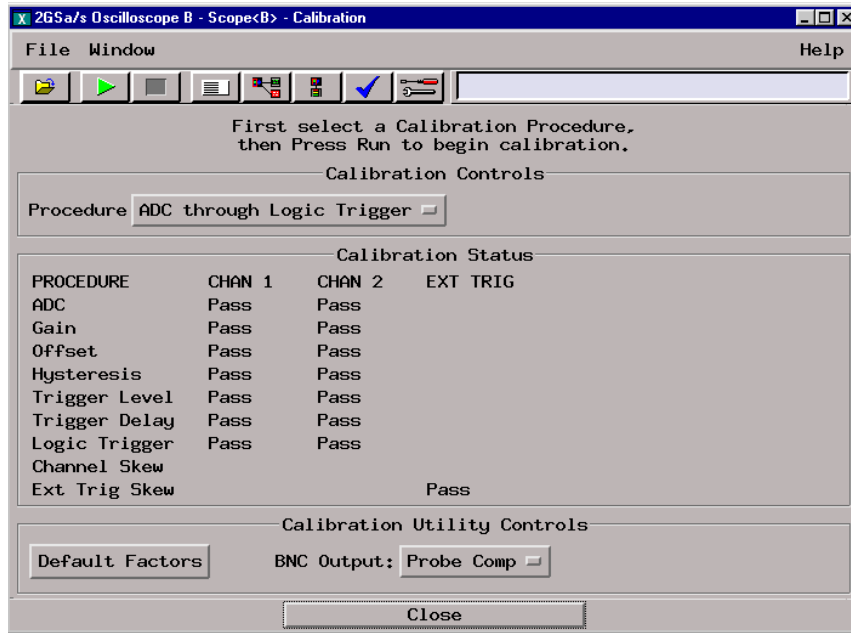


- b Select the BNC Output: field, then select DC Level.
  - c Select the DC volts field, and set it to "0" V.



---

## Verify the cal DC output voltages

- 1 Using the BNC-to-banana adapter, connect the BNC cable between the multimeter and the oscilloscope cal output port.

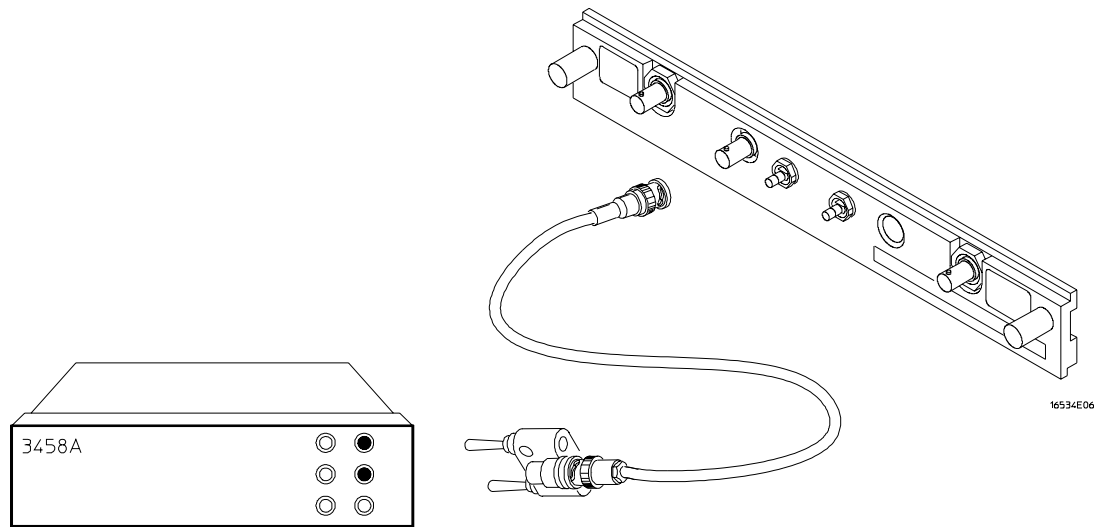

- 2 The digital voltmeter should read close to 0.000 V. Record the reading.  $V_1 = \underline{\hspace{2cm}}$ .
- 3 In the oscilloscope module Calibration window set the DC volts to 5.000 V.
- 4 The digital voltmeter should read close to 5.000 V. Record the reading.  $V_2 = \underline{\hspace{2cm}}$ .
- 5 In the oscilloscope module Calibration window set the DC volts to 2.500 V.
- 6 Subtract  $V_1$  from  $V_2$ . The difference should be close to 5 V.




## Set up the oscilloscope

- 1 In the oscilloscope module Calibration menu, select the BNC Output: field, then select Probe Comp.




- 2 Set up the Channel menu.
  - a In the Logic Analysis window, select the module icon, then select Setup/Display.
  - b Under the Channels tab, select Setup.
  - c Select the Probe field, then enter 1.000:1.
  - d Select Input Z/Coupling: 1M Ohm/DC.

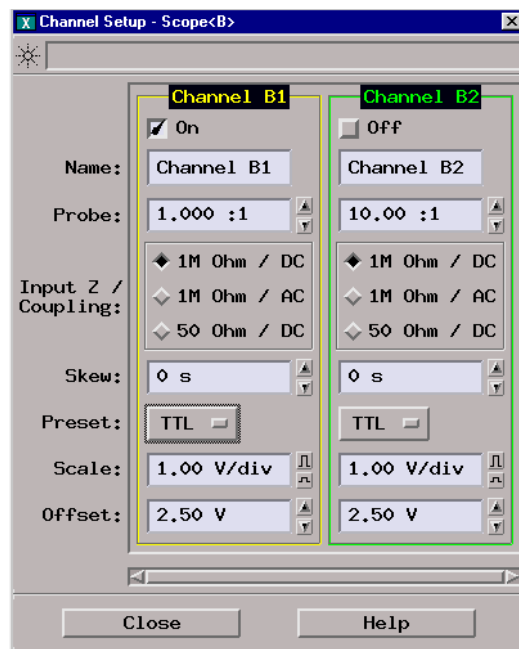

- e Select Close to close the Setup window.

## Verify the AC CAL OUTPUT

- 1 Using the BNC cable, connect channel 1 of the oscilloscope module to the cal output port.
- 2 Select Autoscale. At the popup, select Continue.
- 3 In the oscilloscope Setup window, select the Measure tab. Verify that the waveform is approximately 0.8 V<sub>p\_p</sub> (V<sub>pp</sub>) at approximately 1.0000 KHz (frequency).

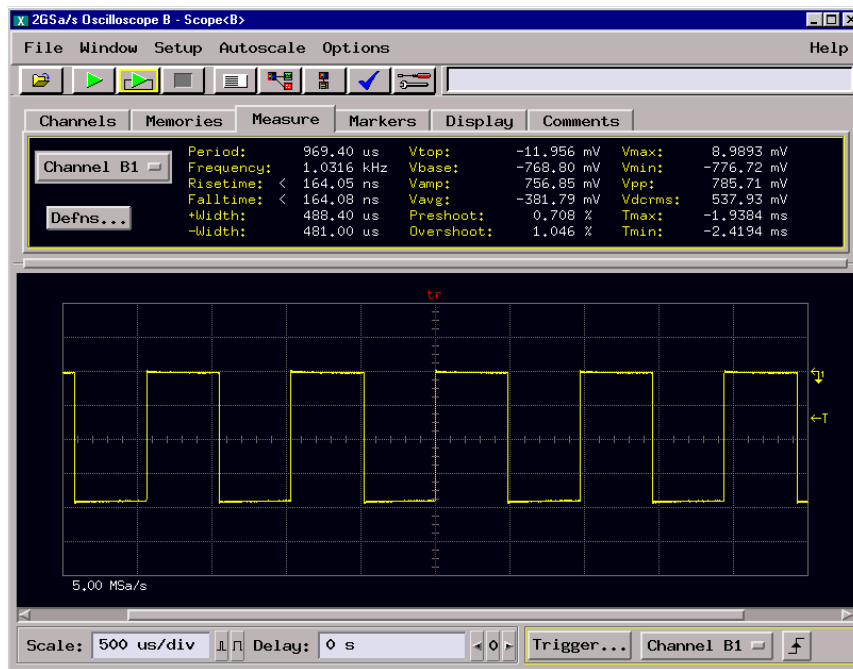

## Replacing Assemblies

- To remove the module 6-2
- To remove the trigger cable 6-3
- To replace the trigger cable 6-4
- To remove the attenuator 6-4
- To replace the attenuator 6-4
- To remove the circuit board 6-5
- To replace the circuit board 6-5
- To replace the module 6-5
- To return assemblies 6-6

---

# Replacing Assemblies

This chapter contains the instructions for removing and replacing the oscilloscope module, the circuit board of the module, the trigger cable, attenuators, and the circuit board. Also in this chapter are instructions for returning assemblies.

---

**CAUTION**

Turn off the instrument before installing, removing, or replacing a module in the instrument. Failure to do so could damage the equipment.

**Tools Required**

A T10 TORX screwdriver is required to remove screws connecting the rear panel to the circuit board.

---

## To remove the module


---

**CAUTION**

Electrostatic discharge can damage electronic components. Use grounded wriststraps and mats when performing any service to this module.

- 1** Remove power from the instrument.
  - a** Exit all logic analysis sessions. In the session manager, select Shutdown.
  - b** At the query, select Power Down.
  - c** When the "OK to power down" message appears, turn the instrument off.
  - d** Disconnect the power cord.
- 2** For multichannel configurations, disconnect the master expander trigger cable.
- 3** Using a T10 TORX screwdriver, loosen the thumb screws.

Starting from the top, loosen the thumb screws on the filler panels and cards located above the module and the thumb screws of the module.

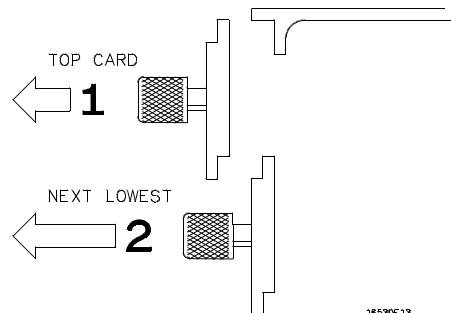

- 4** Starting from the top, pull the cards and filler panels located above the module halfway out.
- 5** If the module consists of a single card, pull the card completely out. Then go to the next page, "To replace the module."


If the module consists of more than one card, pull the complete module approximately halfway out.

- 6** Push all other cards into the card cage, but not completely in.

This is to get them out of the way for removing and replacing the module or a card in the module.

- 7 Starting with the top card in the module, slide the card completely out. Remove each card in the same manner until the faulty card is removed. Then go to the next page, "To replace the module."
  - a If a trigger cable was determined to be faulty, replace the faulty trigger cable on the oscilloscope module (see To remove/replace trigger cable).
  - b If an attenuator was determined to be faulty, replace the faulty attenuator on the oscilloscope module (see To remove/replace Attenuator).
  - c If the oscilloscope module was determined to be faulty, remove the attenuators from the oscilloscope module (see To remove/replace Attenuator), then acquire a replacement oscilloscope module and install the attenuators on the replacement oscilloscope module (see To replace the module).

The remove/replace procedures in this chapter reference the following illustration:

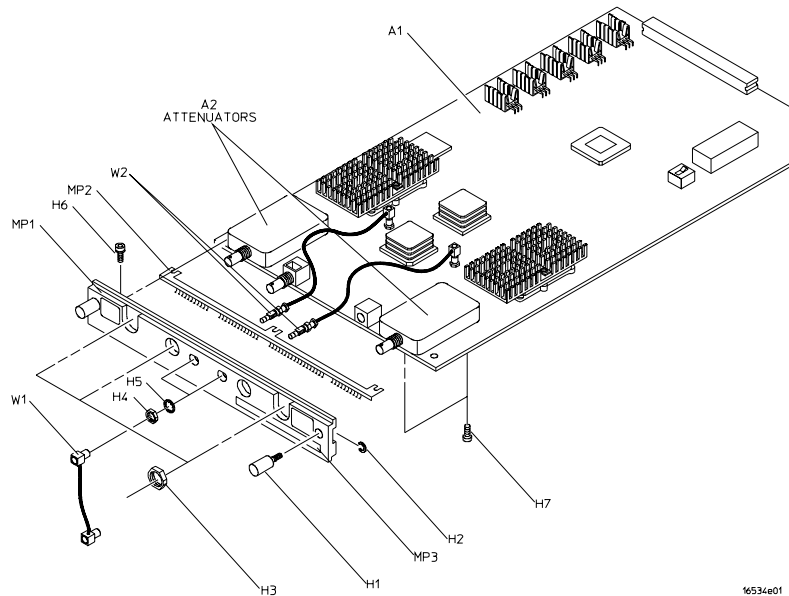

**Exploded view of the Agilent 16533A/34A module.**

## To remove the trigger cable

- 1 Follow the procedures given in "To remove the module" to remove the 16533A/34A oscilloscope module to be serviced.
- 2 Remove the hex nut (H4) and the washer (H5) from the SMB connector on the cable to be removed.
- 3 Pull the straight SMB connector on the cable through the hole in the rear panel.
- 4 Pull the right-angle SMB connector on the cable away from its mating connector on the board.
- 5 Install a new cable (see To replace the trigger cable).

## To replace the trigger cable

- 1 Install the straight SMB connector on the cable through the hole in the rear panel.
  - 2 Attach the washer (H5) and the hex nut (H4) to the straight SMB connector on the cable. Tighten the hex nut.
  - 3 Connect the right-angle SMB connector on the cable to its mating connector on the board.
- 

## To remove the attenuator

- 1 Follow the procedures given in "To remove the module" to remove the 16533A/34A Oscilloscope Module to be serviced.
  - 2 Remove the four hex nuts (H3) from the BNC connectors on the rear panel (MP1).
  - 3 Remove the two hex nuts (H4) and the two washers (H5) from the SMB connectors on the rear panel.
  - 4 Remove the three end plate screws (H6) holding the rear panel (MP1) and the ground spring (MP2) to the board assembly (A1).
  - 5 Pull the rear panel (MP1) and the ground spring (MP2) from the board assembly (A1). You may need to loosen the attenuator retainer screws (H7) before removing the ground spring.
  - 6 Remove the two attenuator retainer screws (H7) holding the attenuator assembly (A2) to the board assembly (A1).
  - 7 Gently pull the attenuator assembly (A2) straight up from the board assembly (A1) being careful not to damage the connector and the components beneath the attenuator assembly.
  - 8 Install a new attenuator assembly (see "To replace the attenuator").
- 

## To replace the attenuator

- 1 Gently push the attenuator assembly (A2) straight down on the board assembly (A1) being careful not to damage the connector and the components beneath the attenuator assembly.
  - 2 Attach the attenuator assembly (A2) to the board assembly (A1) with the two attenuator retainer screws (H7).
  - 3 Assemble the rear panel (MP1) and the ground spring (MP2) to the board assembly (A1) and attach them with the three end plate screws (H6). You may need to loosen the attenuator retainer screws (H7) before assembling the ground spring to the board assembly, then tighten the attenuator screws (H7) when the assembly is finished.
  - 4 Attach the SMB connectors to the rear panel (MP1) with two hex nuts (H4) and two washers (H5).
  - 5 Attach the BNC connectors to the rear panel (MP1) with four hex nuts (H3). Tighten the hex nuts down so that they will not interfere with the installation of the board above the oscilloscope module. One of the flat surfaces on the outside edge of the nut should be parallel with the top edge of the rear panel.
-

---

## To remove the circuit board

- 1 Follow the procedures given in "To remove the module" to remove the 16533A/34A oscilloscope module to be serviced.
- 2 Remove both trigger cables. Follow the procedures given in "To remove the trigger cable".
- 3 Remove both attenuators. Follow the procedures given in "To remove the attenuator".

---


## To replace the circuit board

- 1 Install the attenuators and the rear panel onto the replacement circuit board. Follow the procedures given in "To replace the attenuator".
- 2 Install the trigger cables onto the replacement circuit board. Follow the procedures given in "To replace the trigger cable".

---

## To replace the module

- 1 If the module consists of a single card, slide the card approximately halfway into the mainframe, then go to step 2.  
If the module consists of more than one card, perform the following steps:
  - a Slide the card(s) into the mainframe.  
For multocard configurations, start with the lowest slot position.
  - b Slide the cards above the slots for the module about halfway out of the mainframe.
- 2 Starting with the bottom card, position all cards and filler panels so that the endplates overlap.

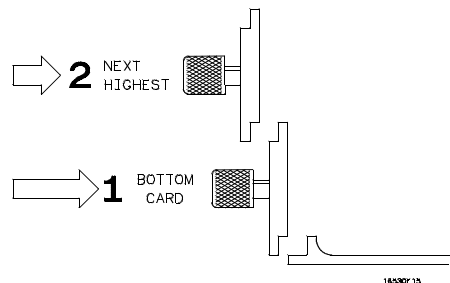

- 3 Seat the cards and hand tighten the thumbscrews. **DO NOT** use the TORX screwdriver to tighten the thumbscrews.

Starting with the bottom card, firmly seat the cards into the backplane connector of the mainframe. Keep applying pressure to the center of the card endplate while tightening the thumbscrews finger-tight. Repeat this for all cards and filler panels starting at the bottom and moving to the top.

---

### CAUTION

For correct air circulation, filler panels must be installed in all unused card slots. Correct air circulation keeps the instrument from overheating. Keep any extra filler panels for future use.

- 4 If a multichannel module is being reconfigured, use the master/expander trigger cable included with the accessory kit of each 16533A/34A card. Starting with the top-most 16533A/34A card, connect the ECL EXT TRIG OUT to the ECL EXT TRIG IN of the card immediately below. Repeat for all cards in the module.
- 

## To return assemblies

Before shipping the module to Agilent Technologies, contact your nearest Agilent Technologies sales office for additional details.

- 1 Write the following information on a tag and attach it to the module.

- Name and address of owner
- Model number
- Serial number
- Description of service required or failure indications

- 2 Remove accessories from the module.

Only return accessories to Agilent Technologies if they are associated with the failure symptoms.

- 3 Package the module.

You can use either the original shipping containers, or order materials from an Agilent Technologies sales office.

---

**CAUTION**

Electrostatic discharge can damage electronic components. For protection against electrostatic discharge, package the module in electrostatic material.

- 4 Seal the shipping container securely, and mark it FRAGILE.



Replaceable Parts  
Replaceable Parts Ordering 7-2  
Replaceable Parts List 7-3  
Exploded View 7-5

---

# Replaceable Parts

This chapter contains information for identifying and ordering replaceable parts for your oscilloscope.

---

## Replaceable Parts Ordering

### **Parts listed**

To order a part on the list of replaceable parts, quote the Agilent Technologies part number, indicate the quantity desired, and address the order to the nearest Agilent Technologies Sales Office.

### **Parts not listed**

To order a part not on the list of replaceable parts, include the model number and serial number of the module, a description of the part (including its function), and the number of parts required. Address the order to your nearest Agilent Technologies Sales Office.

### **Direct mail order system**

To order using the direct mail order system, contact your nearest Agilent Technologies Sales Office.

Within the USA, Agilent Technologies can supply parts through a direct mail order system. The advantages to the system are direct ordering and shipment from the Agilent Technologies Part Center in Mountain View, California. There is no maximum or minimum on any mail order. (There is a minimum amount for parts ordered through a local Agilent Technologies Sales Office when the orders require billing and invoicing.) Transportation costs are prepaid (there is a small handling charge for each order) and no invoices.

In order for Agilent Technologies to provide these advantages, a check or money order must accompany each order. Mail order forms and specific ordering information are available through your local Agilent Technologies Sales Office. Addresses and telephone numbers are located in a separate document at the back of the service guide.

### **Exchange Assemblies**

Some assemblies are part of an exchange program with Agilent Technologies.

The exchange program allows you to exchange a faulty assembly with one that has been repaired and performance verified by Agilent Technologies.

After you receive the exchange assembly, return the defective assembly to Agilent Technologies. A United States customer has 30 days to return the defective assembly. If you do not return the defective assembly within the 30 days, Agilent Technologies will charge you an additional amount. This amount is the difference in price between a new assembly and that of the exchange assembly. For orders not originating in the United States, contact your nearest Agilent Technologies Sales Office for information.

### **See Also**

"To return assemblies," in chapter 6.

---

## Replaceable Parts List

The replaceable parts list is organized by reference designation and shows exchange assemblies, electrical assemblies, then other parts.

The exploded view does not show all of the parts in the replaceable parts list.

Information included for each part on the list consists of the following:

- Reference designator
- Agilent Technologies part number
- Total quantity included with the instrument (Qty)
- Description of the part

Reference designators used in the parts list are as follows:

- A Assembly
- H Hardware
- MP Mechanical Part
- W Cable

Replaceable Parts  
**Replaceable Parts List**

---


**16533A/34A Replaceable Parts**

---

<b>Ref. Des.</b>	<b>Agilent Part Number</b>	<b>QTY</b>	<b>Description</b>
<b>Exchange Assembly</b>			
	16533-69504	1	16533A Exchange Circuit Board (does not include attenuator assemblies)
	16534-69504	1	16534A Exchange Circuit Board (does not include attenuator assemblies)
	16534-69401		Exchange Attenuator
<b>Replacement Parts</b>			
A1	16534-66504	1	16534A Circuit Board Assembly (does not include attenuator assemblies)
A1	16533-66504	1	16533A Circuit Board Assembly (does not include attenuator assemblies)
A2	16534-63401	2	Attenuator Assembly
H1	16500-22401	2	Rear Panel Thumbscrew
H2	0510-0684	2	Thumbscrew Retaining Ring
H3	1250-2075	3	Nut, Hex, 1/2-inch RF Connector
H4	0515-0430	3	Rear Panel Screw
H5	0515-1246	4	Attenuator Retainer Screw
MP1	16500-29101	1	Ground Spring
MP2	16534-40501	1	Rear Panel
MP3	16534-94301	1	ID Label (16534A)
MP3	16533-94301	1	ID Label (16533A)
MP4	16534-94302	1	CAL/PWR Label
MP5	16532-94302	1	Warning Label
MP6	1401-0260	1	Vinyl Molded Cap
MP7	16534-44701	3	Circuit Board Spacer
W1	16532-61601	1	Master/Expander Trigger Cable
W2	16532-61602	2	External Trigger Cable

---

Exploded View

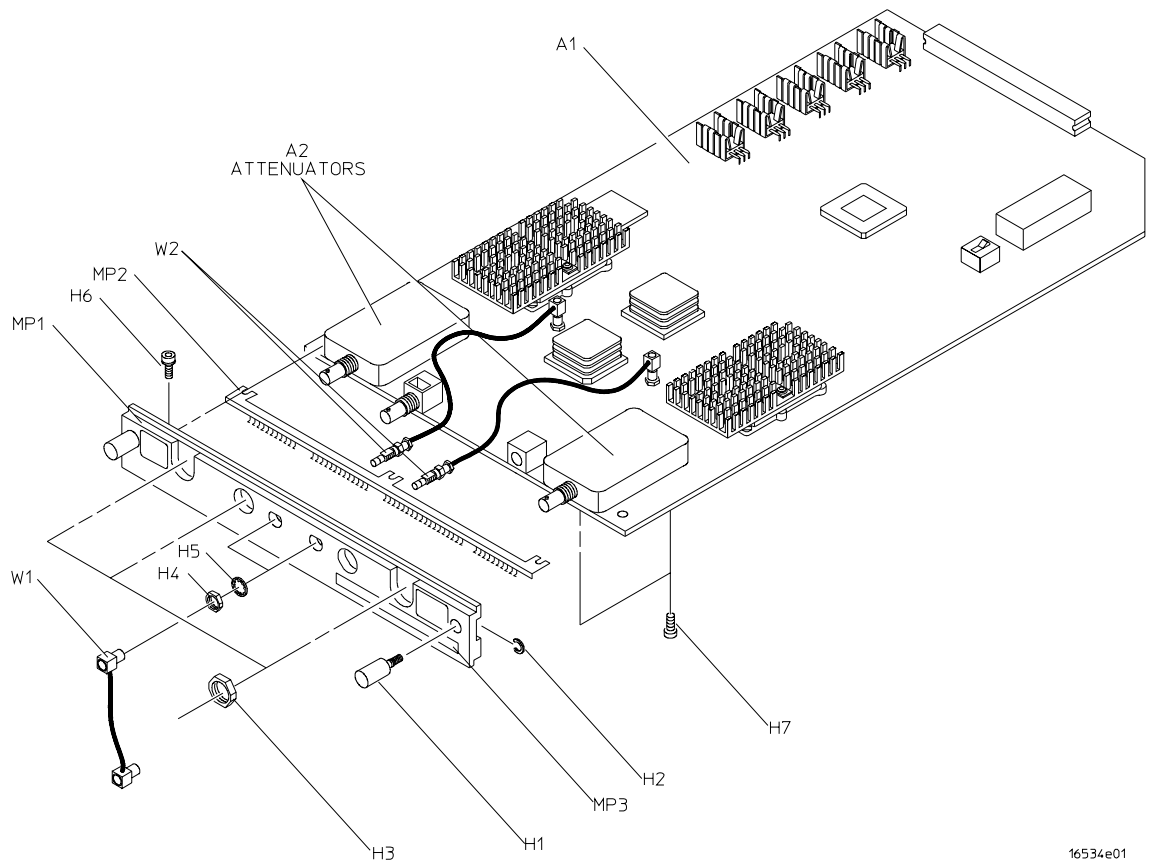

16534e01

Exploded view of the 16533A/34A module



Theory of Operation  
Block-Level Theory 8-3  
Self-Tests Description 8-7  
    Oscilloscope Tests (Scope PV) 8-7


---

# Theory of Operation

This chapter tells the theory of operation for the oscilloscope and describes the self-tests. The information in this chapter is to help you understand how the oscilloscope operates and what the self-tests are testing. This information is not intended for component-level repair.



# Block-Level Theory

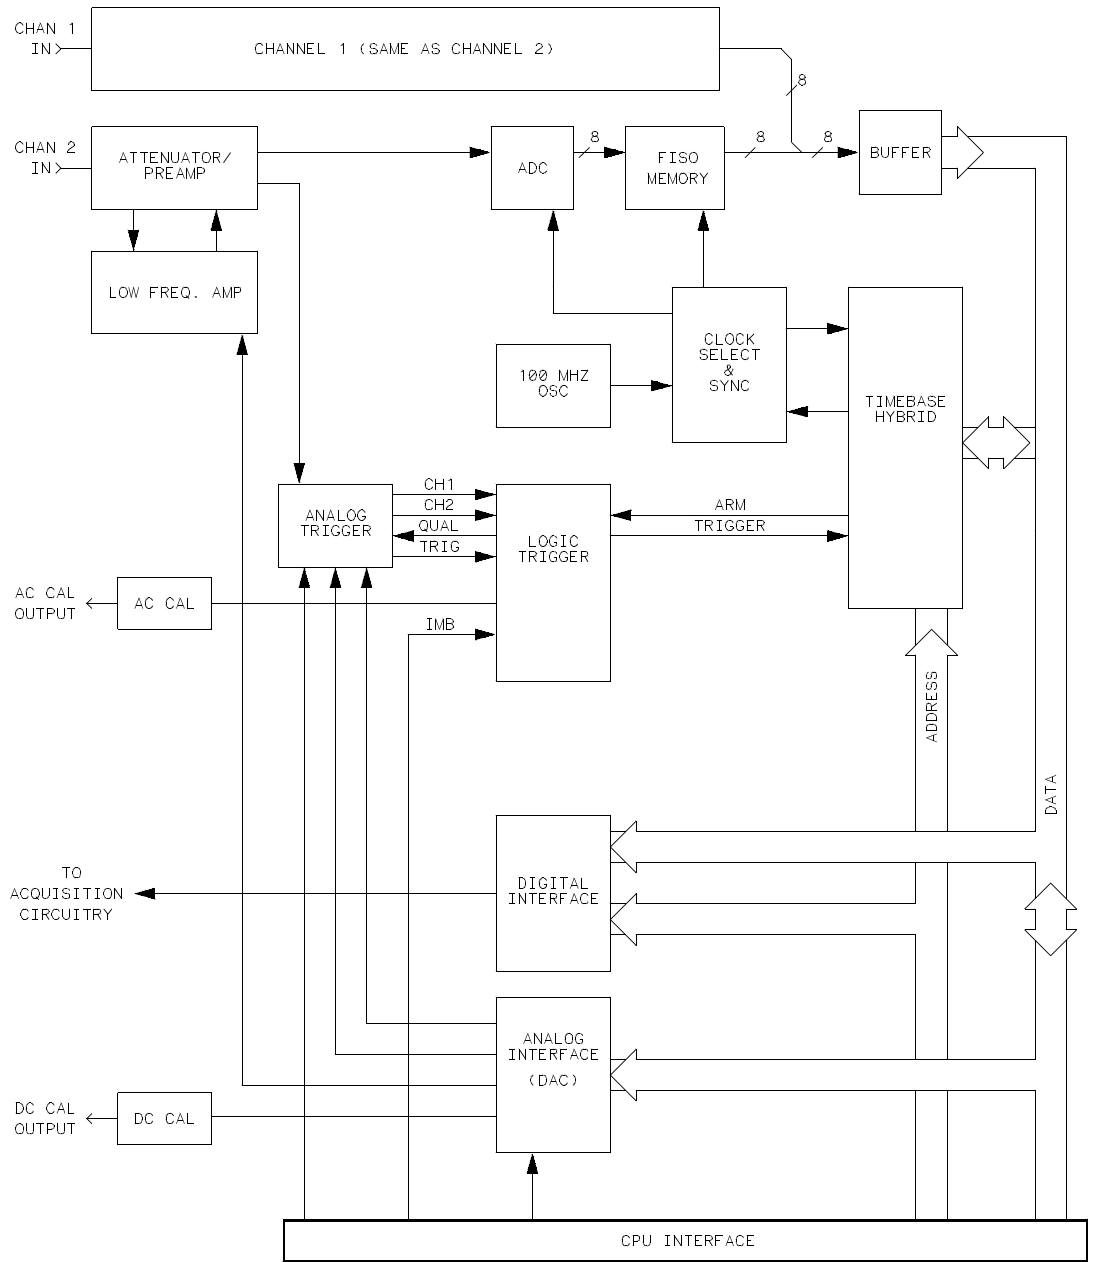

16532B 14

## The Oscilloscope Board

## Oscilloscope Board Theory

The following paragraphs contain block level theory of operation. This theory is not intended for component level troubleshooting, rather it is to be used to help isolate a module failure to card level.

The 16533A/34A Oscilloscope Module is contained on one board. It runs at a 2 GSa/s digitizing rate (16534A) and 1GSa/s digitizing rate (16533A), with a 500 MHz single-shot (real-time) bandwidth (16534A) and 250 MHz single-shot (real-time) bandwidth (16533A), 32,768 samples per measurement per channel, with 2-channel simultaneous acquisition which is expandable to up to 8 channels.

### **Attenuator Theory**

The channel input signals are conditioned by the attenuator/preamps, thick film hybrids containing passive attenuators, an impedance converter, and a programmable amplifier. The channel sensitivity, as displayed, defaults to the standard 1-2-5 sequence (other calibrated sensitivities can also be set). However, the firmware uses two passive attenuators, 5:1 and 25:1 to get attenuations of 1:1, 5:1, 25:1, and 125:1. With the attenuation and programmable gain of the amplifier the entire sensitivity range is calibrated. (On ranges below 7 mV/div, the firmware expands the signal digitally.)

The input has a selectable 1 M $\Omega$  or 50  $\Omega$  input impedance. Compensation for the passive attenuators is laser trimmed and not adjustable. After the passive attenuators, the signal is split into high-frequency and low-frequency components. Low-frequency components are amplified on the main assembly where they are combined with the offset voltage. The ac coupling and low-frequency reject are implemented in the low-frequency amplifier.

The high- and low-frequency components of the signal are recombined and applied to the input FET of the preamp. The FET provides a high impedance load for the input attenuators and a low impedance drive for the preamp. The programmable preamp adjusts the gain to suit the required sensitivity and provides two output signals to the Main assembly. One signal is the same phase as the input and goes to the trigger circuitry. The other is of opposite phase and is sent to the ADC hybrid.

### **Oscilloscope Acquisition**

The acquisition circuitry provides the sampling, digitizing, and storing of the signals from the channel attenuators. The channels are identical. The external trigger (ECL) input cannot be displayed. Trigger signals from each channel and the external triggers synchronize acquisition through the time base circuitry. A 100 MHz oscillator and a time base provide system timing and sample clocking. A voltage-controlled oscillator (VCO), frequency divider, and digital phase detector provide the sample clock for higher sample rates. After conditioning and sampling, the signals are digitized, then stored in a hybrid IC containing a FISO (fast in, slow out) memory.

**ADC Hybrid** The ADC hybrid provides all of the sampling, digitizing, and high-speed waveform storage. The ADC includes a phase-locked loop frequency converter that, for sample rates from 250 MHz to 2 GHz, multiplies the input clock from the time base.

**FISO Memory** 32,768 samples of the FISO (fast in, slow out) memory are used per measurement per channel. Memory positions are not addressed directly. The configuration is a ring which loops continuously as it is clocked. Memory position is tracked by counting clocks. The clocking rate is the same as the ADC, however the clock

frequency is half that of the ADC since the FISO clocks on both transitions of the clock period. Data is buffered onto the CPU data bus for processing.

**Triggering** There are two main trigger circuits that trigger four trigger sources. The two trigger circuits are the analog trigger and the logic trigger. The analog trigger IC operates as a multichannel Schmidt trigger/comparator. A trigger signal (a copy of the analog input signal) from each of the inputs is directed to the analog trigger IC inputs. The trigger signal is continuously compared with the trigger reference level selected by the user. Once the trigger condition is met, the trigger TRUE signal is fed to the logic trigger, which begins the acquisition and store functions by way of the time base.

The four trigger sources are Channel 1, Channel 2, Intermodule Bus (IMB), and external BNC. The operation of the input channels was discussed previously. The IMB trigger signal is sent directly to the logic trigger. External triggering is provided by the BNC input of the 16500B Logic Analysis System mainframe.

**Time Base** The time base provides the sample clocks and timing necessary for data acquisition. It consists of the 100 MHz reference oscillator and time base hybrid.

The 100 MHz reference oscillator provides the base sample frequency.

The time base hybrid has programmable dividers to provide the rest of the sample frequencies appropriate for the time range selected. The time base uses the time-stretched output of the fine interpolator to time-reference the sampling to the trigger point. The time base has counters to control how much data is taken before (pre-trigger data) and after (post-trigger data) the trigger event. After the desired number of pre-trigger samples has occurred, the Time base hybrid sends a signal to the Logic Trigger (trigger arm) indicating it is ready for the trigger event. When the trigger condition is satisfied, the Logic Trigger sends a signal back to the time base hybrid. The time base hybrid then starts the post-trigger delay counter.

When the countdown reaches zero, the sample clocks are stopped and the CPU is signaled that the acquisition is complete. The Fine Interpolator is a dual-slope integrator that acts as a time-interval stretcher. When the logic trigger receives a signal that meets the programmed triggering requirements, it signals the time base. The time base then sends a pulse to the fine interpolator. The pulse is equal in width to the time between the trigger and the next sample clock. The fine interpolator stretches this time by a factor of approximately 500. Meanwhile, the time base hybrid runs a counter with a clock derived from the sample rate oscillator. When the interpolator indicates the stretch is complete, the counter is stopped. The count represents, with much higher accuracy, the time between the trigger and the first sample clock. The count is stored and used to place the recently acquired data in relationship with previous data.

**AC Cal** The AC Cal is a multiplexer circuit that provides several signals to the Probe Compensation/AC Calibrator outputs. The signal provided depends on the mode of the instrument. It provides a probe compensation signal, a pulse representing the trigger event, or signals used for self-calibration. The probe compensation signal is derived from the real-time clock oscillator and can be set from 250 mHz to approximately 32 kHz. The AC cal is sent through an analog multiplexer to the front panel for probe compensation.

**DC Cal** The DC Cal output, a rear panel signal, is used for self-calibration. It is one output from the 16-channel DAC.

**Digital Interface** The Digital Interface provides control and interface between the system control and digital functions in the acquisition circuitry.

**Analog Interface** The Analog Interface provides analog control of functions in the acquisition circuitry. It is primarily a 16-channel DAC with an accurate reference and filtered outputs. The analog interface controls:

- Channel offsets
- Trigger levels
- Two logic trigger functions
- The DC Cal output for instrument and probe calibration

---

# Self-Tests Description

The self-tests identify the correct operation of major functional areas in the oscilloscope. The self-tests are not intended for component-level diagnostics.

---

## Oscilloscope Tests (PV)

The following self-tests check the major components of the 16533A/34A oscilloscope module as well as all associated circuitry. When the self-tests have all been completed with a "PASS" status, the major data and control pipelines in the 16533A/34A oscilloscope module are functioning properly.

**Test FISO** This test verifies the correct operation of the FISO (fast-in/slow-out) data memory on the board. Test patterns are written into the memory and then read and compared with known values.

**Test ADC** This test verifies the correct operation of the A/D convertor on the board. A check of the trigger in Trigger Immediate mode is first made. The A/D convertors are then exercised by setting the reference voltage and channel offset such that a simulated acquisition obtains data in the extremes and middle of the quantization range of the A/D convertor. After each simulated acquisition, the data is compared with known values.

**Test DAC** This test verifies the correct operation of the D/A convertor on the board. Both the offset and trigger level D/A convertors for each channel are set to a reference level and then changed. The logic trigger IC is programmed to detect the changes. The detection of a correct trigger indicates that the D/A convertor is operating normally.

**Test Logic Trigger** This test verifies the correct operation of the trigger components on the board. First, the logic trigger memory is checked by writing and then reading known patterns. The logic qualifiers, logic trigger output, and trigger holdoff are then checked.

**Test Timebase** The pre-trigger and post-trigger delay modes are first tested by programming a predetermined time interval in the trigger counters. At the end of the time intervals, the arm, trigger, and run status bits are read and compared with known values. The coarse and fine interpolators are then checked by reading the values of the interpolator counters after a simulated acquisition. The counter values are then compared with a known value. Finally, the sample clock is checked by programming a sample clock frequency and then reading the status of the clock to detect when one clock period has elapsed. The clock period time interval is then compared with a known value.

**Test IMB** This test verifies the correct operation of the oscilloscope board interface to the intermodule bus.

**Test All** This will automatically execute each test, one at a time, until all tests are done.



Reproduction, adaptation, or translation without prior written permission is prohibited, except as allowed under the copyright laws.

#### Document Warranty

The information contained in this document is subject to change without notice.

**Agilent Technologies makes no warranty of any kind with regard to this material, including, but not limited to, the implied warranties or merchantability and fitness for a particular purpose.**

Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Complete product warranty information is given at the end of this manual.

#### Safety

This apparatus has been designed and tested in accordance with IEC Publication 348, Safety Requirements for Measuring Apparatus, and has been supplied in a safe condition. This is a Safety Class I instrument (provided with terminal for protective earthing). Before applying power, verify that the correct safety precautions are taken (see the following warnings). In addition, note the external markings on the instrument that are described under "Safety Symbols."

#### Warning

- Before turning on the instrument, you must connect the protective earth terminal of the instrument to the protective conductor of the (mains) power cord. The mains plug shall only be inserted in a socket outlet provided with a protective earth contact. You must not negate the protective action by using an extension cord (power cable) without a protective conductor (grounding). Grounding one conductor of a two-conductor outlet is not sufficient protection.
- Only fuses with the required rated current, voltage, and specified type (normal blow, time delay, etc.) should be used. Do not use repaired fuses or short-circuited fuseholders. To do so could cause a shock of fire hazard.

- Service instructions are for trained service personnel. To avoid dangerous electric shock, do not perform any service unless qualified to do so. Do not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present.

- If you energize this instrument by an auto transformer (for voltage reduction), make sure the common terminal is connected to the earth terminal of the power source.
- Whenever it is likely that the ground protection is impaired, you must make the instrument inoperative and secure it against any unintended operation.
- Do not operate the instrument in the presence of flammable gasses or fumes. Operation of any electrical instrument in such an environment constitutes a definite safety hazard.
- Do not install substitute parts or perform any unauthorized modification to the instrument.
- Capacitors inside the instrument may retain a charge even if the instrument is disconnected from its source of supply.
- Use caution when exposing or handling the CRT. Handling or replacing the CRT shall be done only by qualified maintenance personnel.

#### Safety Symbols



Instruction manual symbol: the product is marked with this symbol when it is necessary for you to refer to the instruction manual in order to protect against damage to the product.



Hazardous voltage symbol.



Earth terminal symbol: Used to indicate a circuit common connected to grounded chassis.

#### WARNING

The Warning sign denotes a hazard. It calls attention to a procedure, practice, or the like, which, if not correctly performed or adhered to, could result in personal injury. Do not proceed beyond a Warning sign until the indicated conditions are fully understood and met.

#### CAUTION

The Caution sign denotes a hazard. It calls attention to an operating procedure, practice, or the like, which, if not correctly performed or adhered to, could result in damage to or destruction of part or all of the product. Do not proceed beyond a Caution symbol until the indicated conditions are fully understood or met.

---

**Product Warranty**

This Agilent Technologies product has a warranty against defects in material and workmanship for a period of one year from date of shipment. During the warranty period, Agilent Technologies will, at its option, either repair or replace products that prove to be defective.

For warranty service or repair, this product must be returned to a service facility designated by Agilent Technologies.

For products returned to Agilent Technologies for warranty service, the Buyer shall prepay shipping charges to Agilent Technologies and Agilent Technologies shall pay shipping charges to return the product to the Buyer. However, the Buyer shall pay all shipping charges, duties, and taxes for products returned to Agilent Technologies from another country.

Agilent Technologies warrants that its software and firmware designated by Agilent Technologies for use with an instrument will execute its programming instructions when properly installed on that instrument. Agilent Technologies does not warrant that the operation of the instrument software, or firmware will be uninterrupted or error free.

**Limitation of Warranty**

The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by the Buyer, Buyer-supplied software or interfacing, unauthorized modification or misuse, operation outside of the environmental specifications for the product, or improper site preparation or maintenance.

No other warranty is expressed or implied. Agilent Technologies specifically disclaims the implied warranties or merchantability and fitness for a particular purpose.

**Exclusive Remedies**

The remedies provided herein are the buyer's sole and exclusive remedies. Agilent Technologies shall not be liable for any direct, indirect, special, incidental, or consequential damages, whether based on contract, tort, or any other legal theory.

**Assistance**

Product maintenance agreements and other customer assistance agreements are available for Agilent Technologies products.

For any assistance, contact your nearest Agilent Technologies Sales Office.

**Certification**

Agilent Technologies certifies that this product met its published specifications at the time of shipment from the factory. Agilent Technologies further certifies that its calibration measurements are traceable to the United States National Institute of Standards and Technology, to the extent allowed by the Institute's calibration facility, and to the calibration facilities of other International Standards Organization members.

**About this edition**

This is the second edition of the *Agilent Technologies 16533A/34A Digitizing Oscilloscope Service Guide*.

Publication number 16534-97013

Printed in USA.

Edition dates are as follows:

First edition, August 1995

Second edition, January 2000

Third edition, September 2000

New editions are complete revisions of the manual. Update packages, which are issued between editions, contain additional and replacement pages to be merged into the manual by you. The dates on the title page change only when a new edition is published.

A software or firmware code may be printed before the date. This code indicates the version level of the software or firmware of this product at the time the manual or update was issued. Many product updates do not require manual changes; and, conversely, manual corrections may be done without accompanying product changes. Therefore, do not expect a one-to-one correspondence between product updates and manual updates.

The following list of pages gives the date of the current edition and of any changed pages to that edition.

All pages original edition.